

FIG. 1

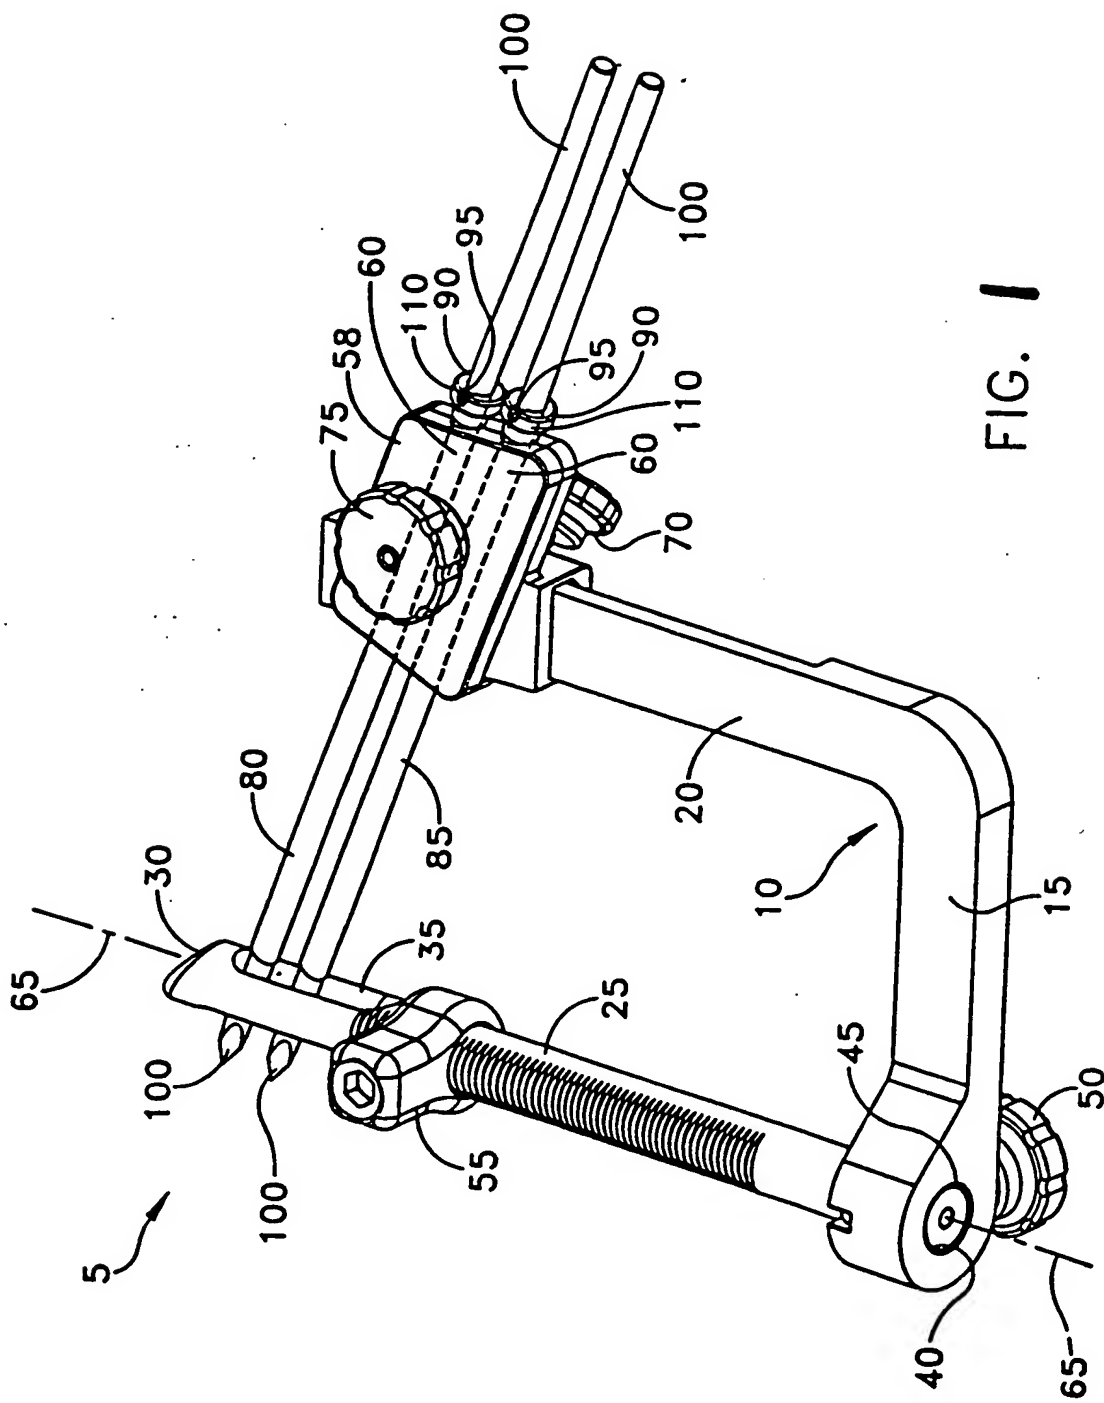


FIG. 1

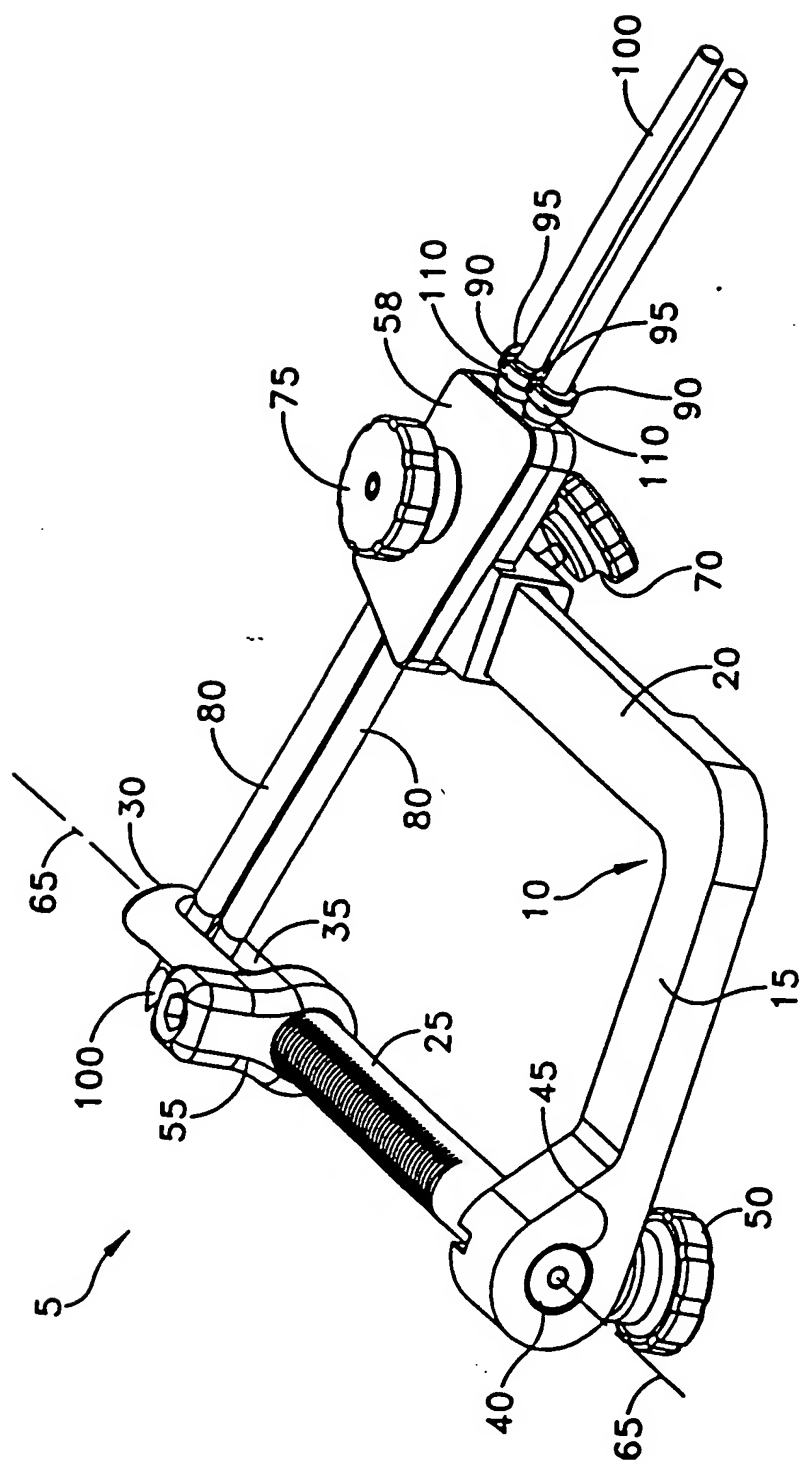


FIG. 2

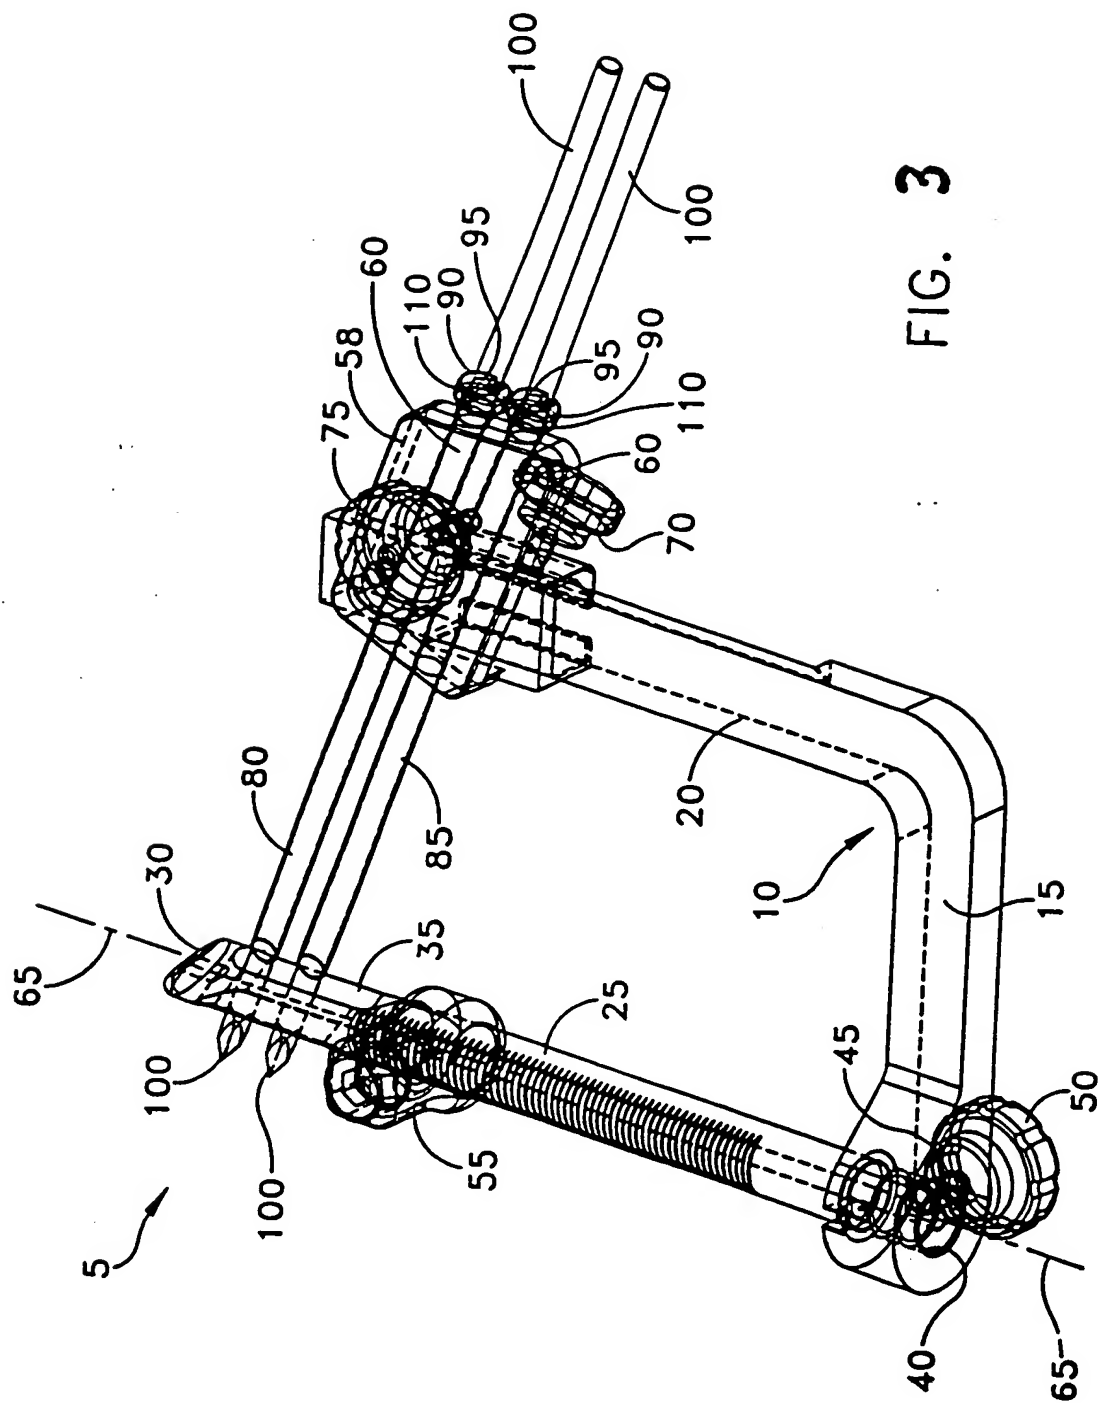


FIG. 3

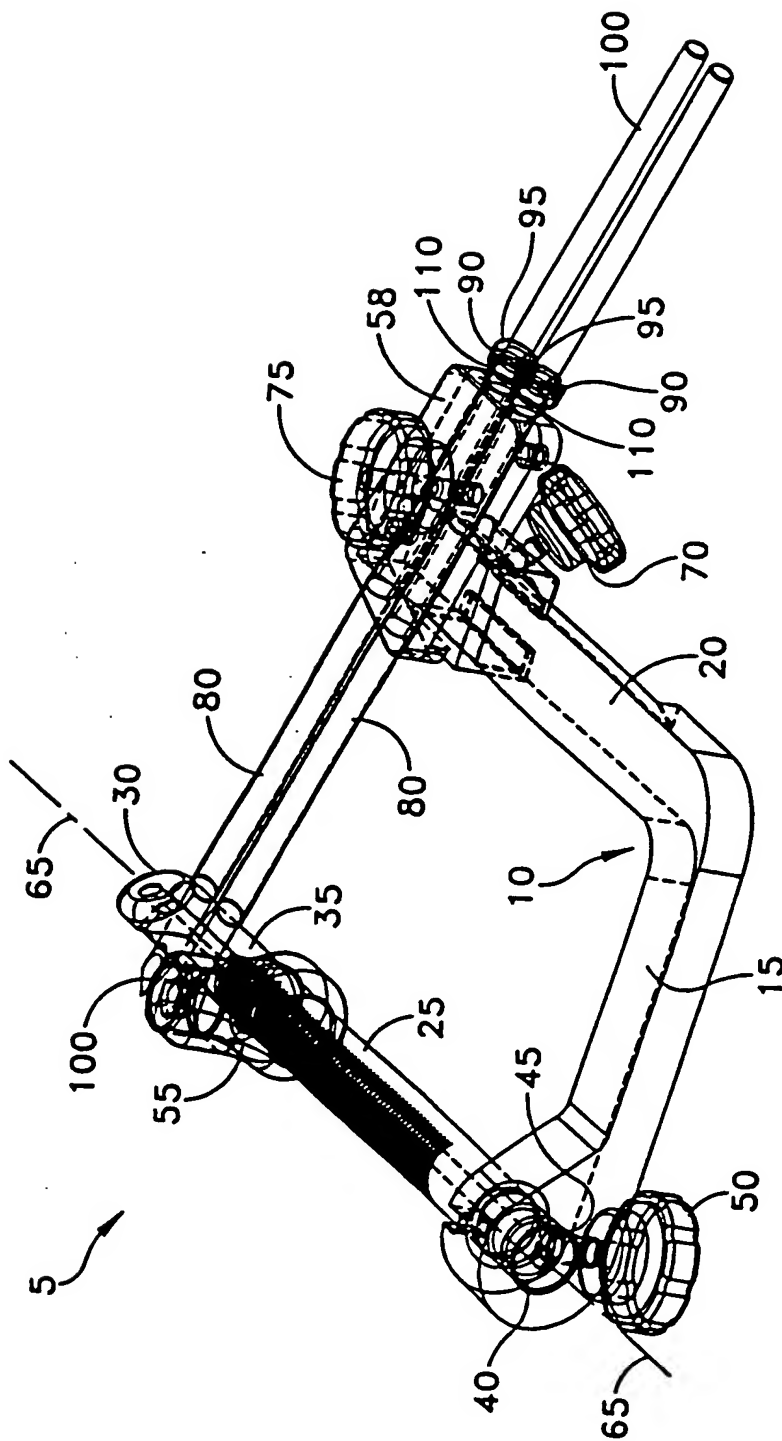


FIG. 4

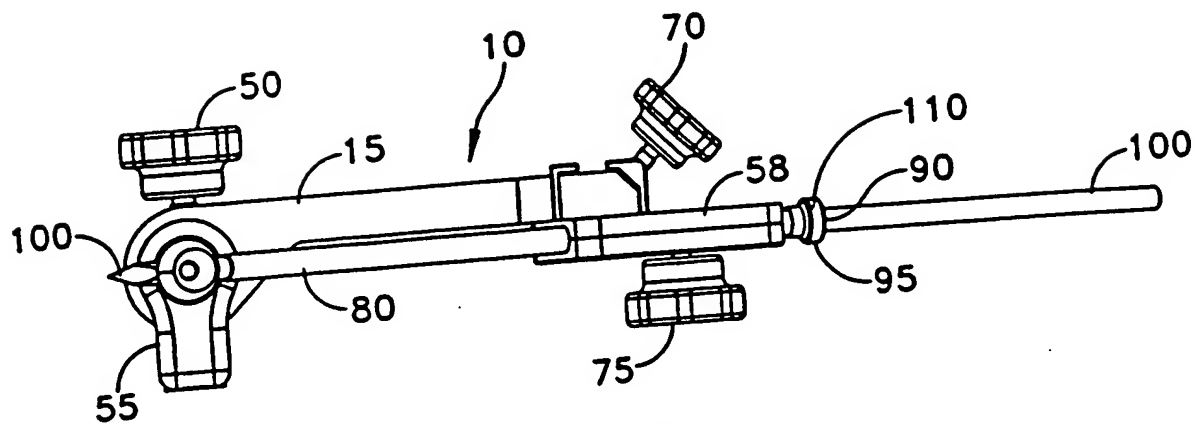


FIG. 7

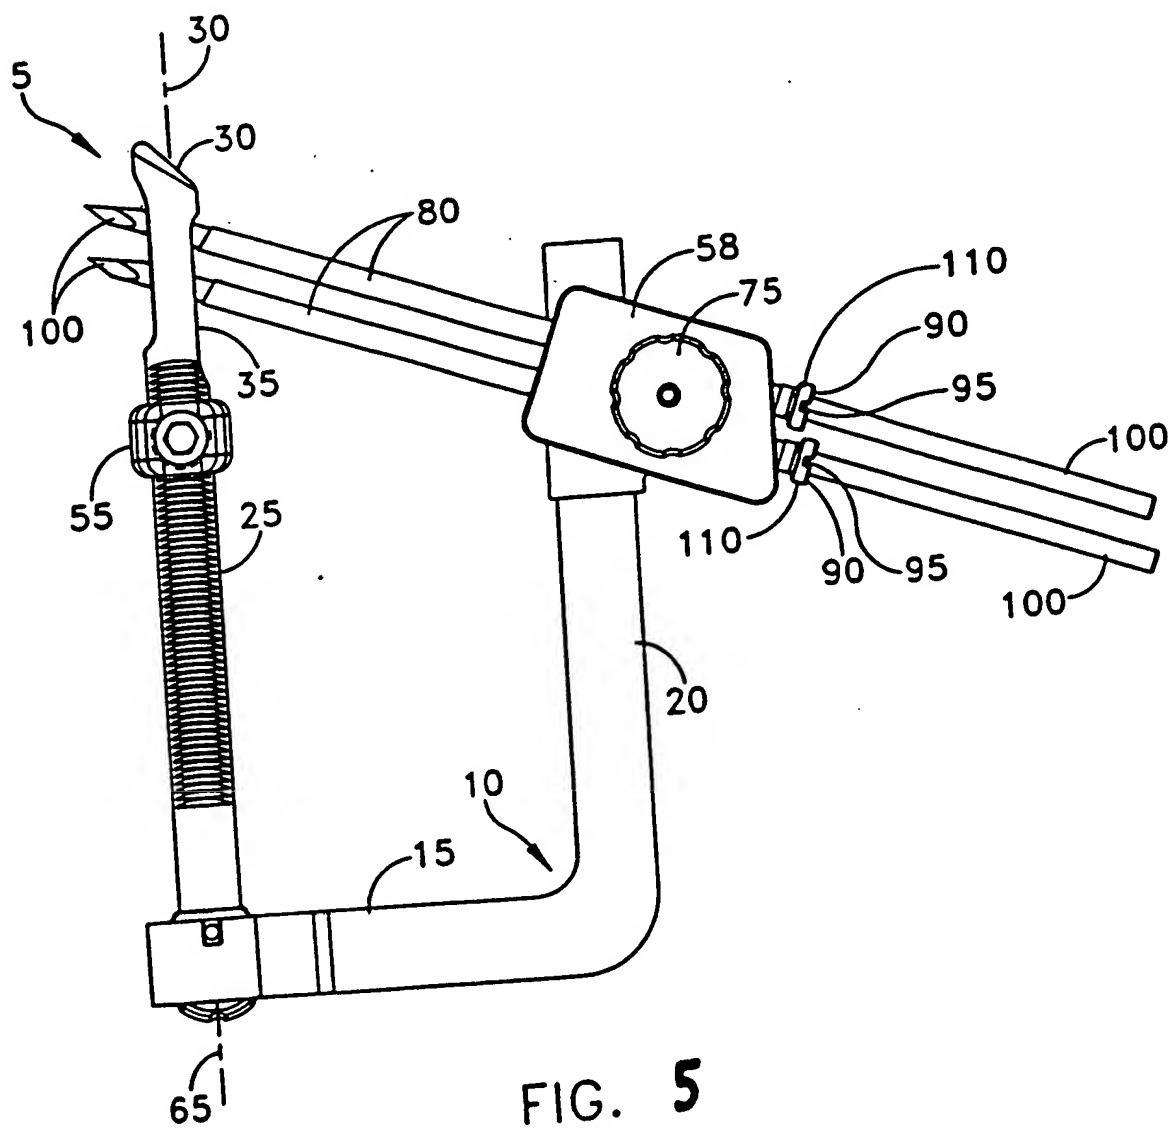


FIG. 5

10039857, 102601

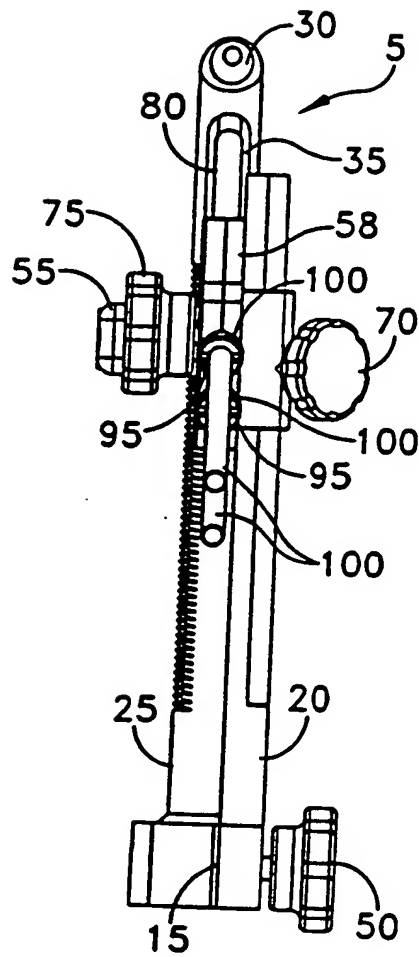


FIG. 6

FIG. 8

10039857-102604

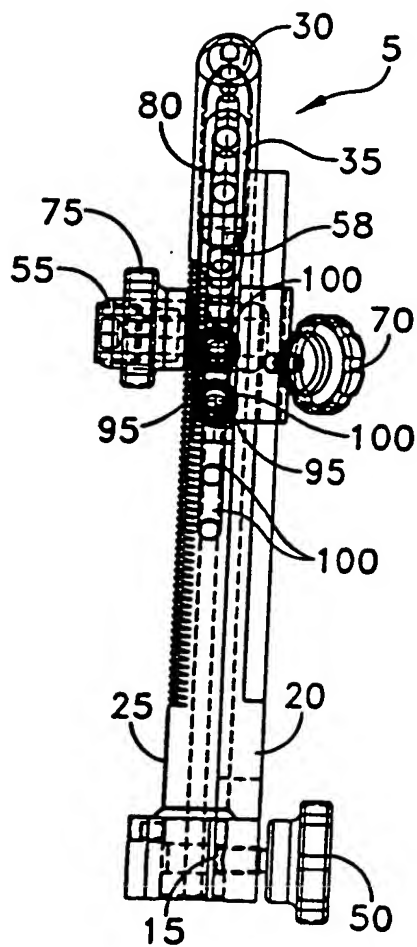


FIG. 9



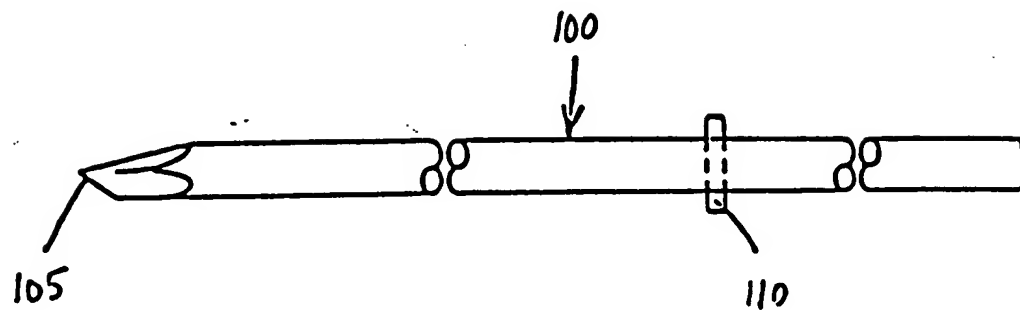


FIG. 12

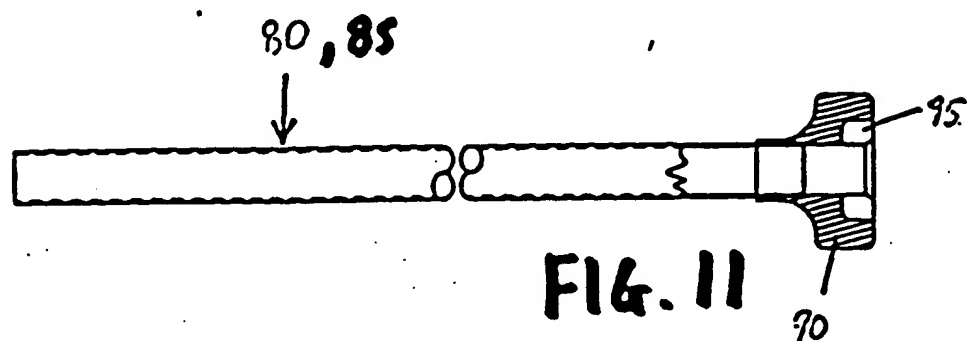


FIG. 11

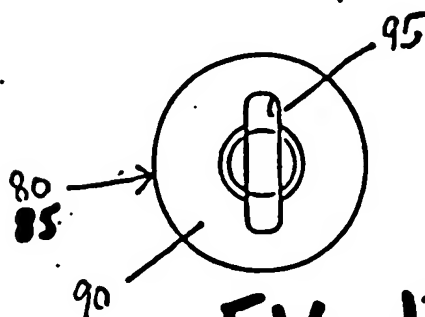


FIG. 13

10039857402501

10039857-102601

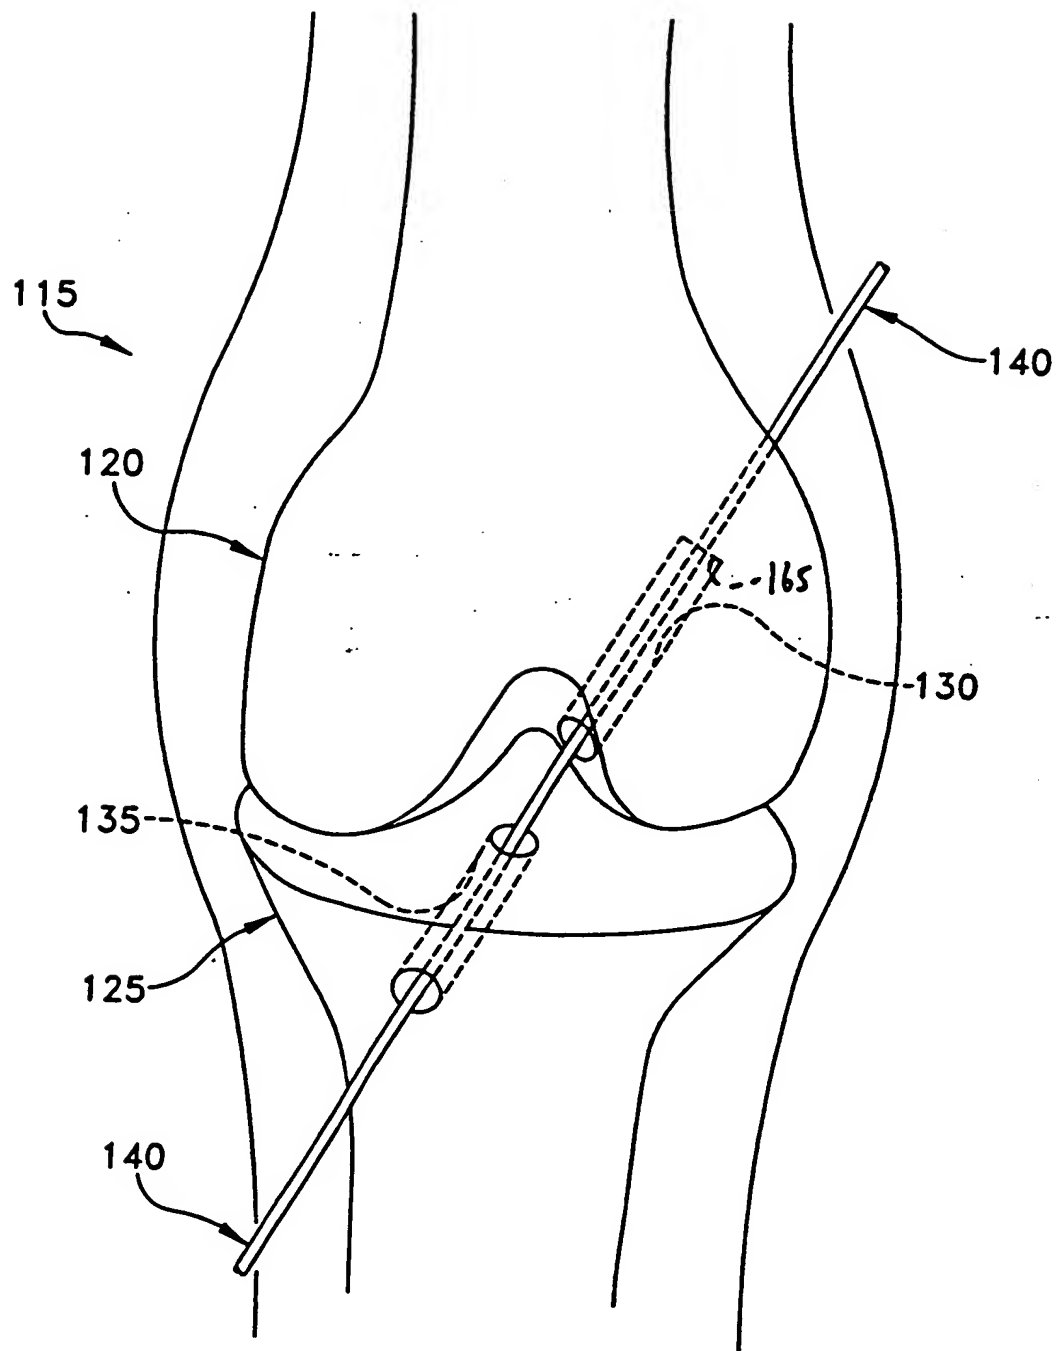


FIG. 14

10039857-10601

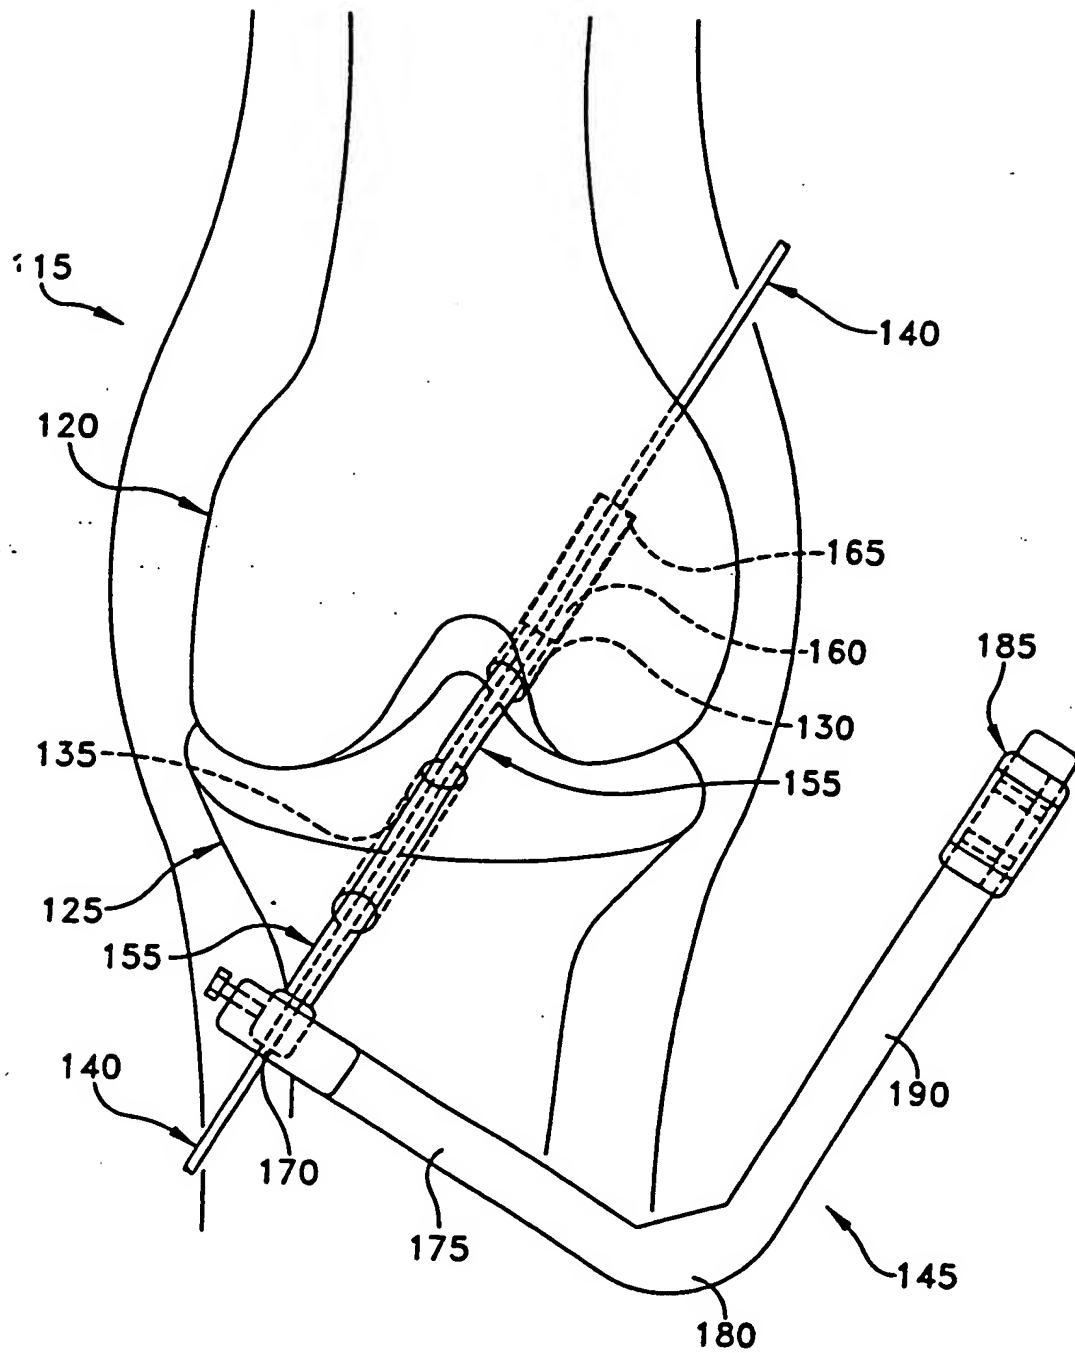


FIG. 15

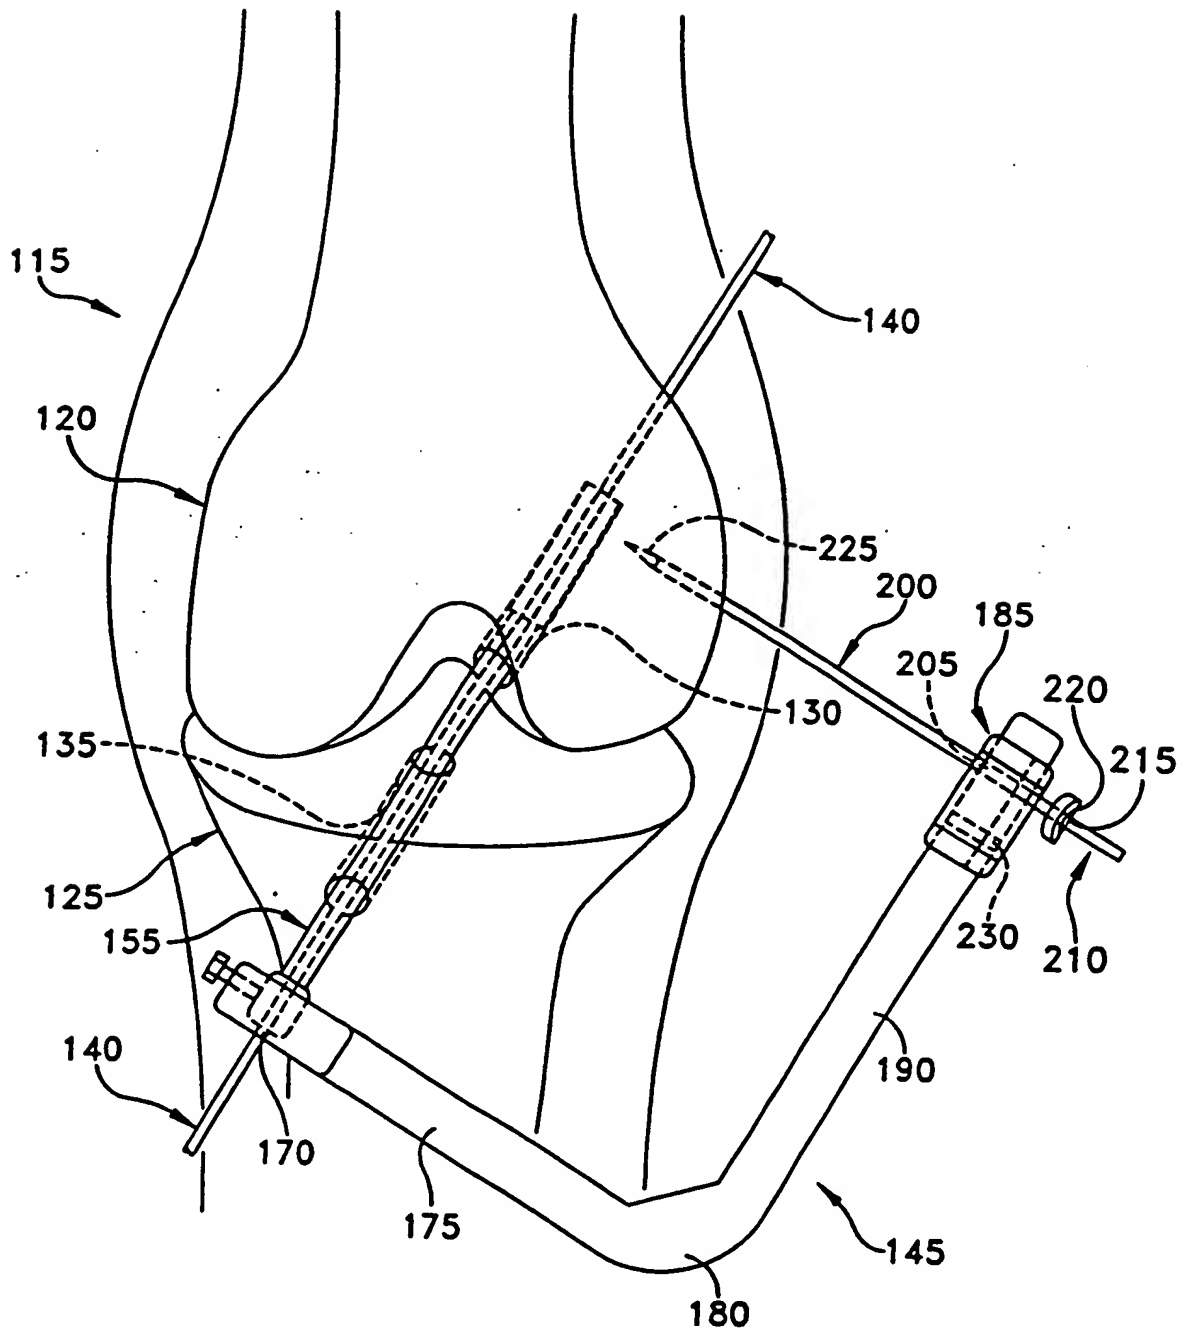


FIG. 16

FIG. 17

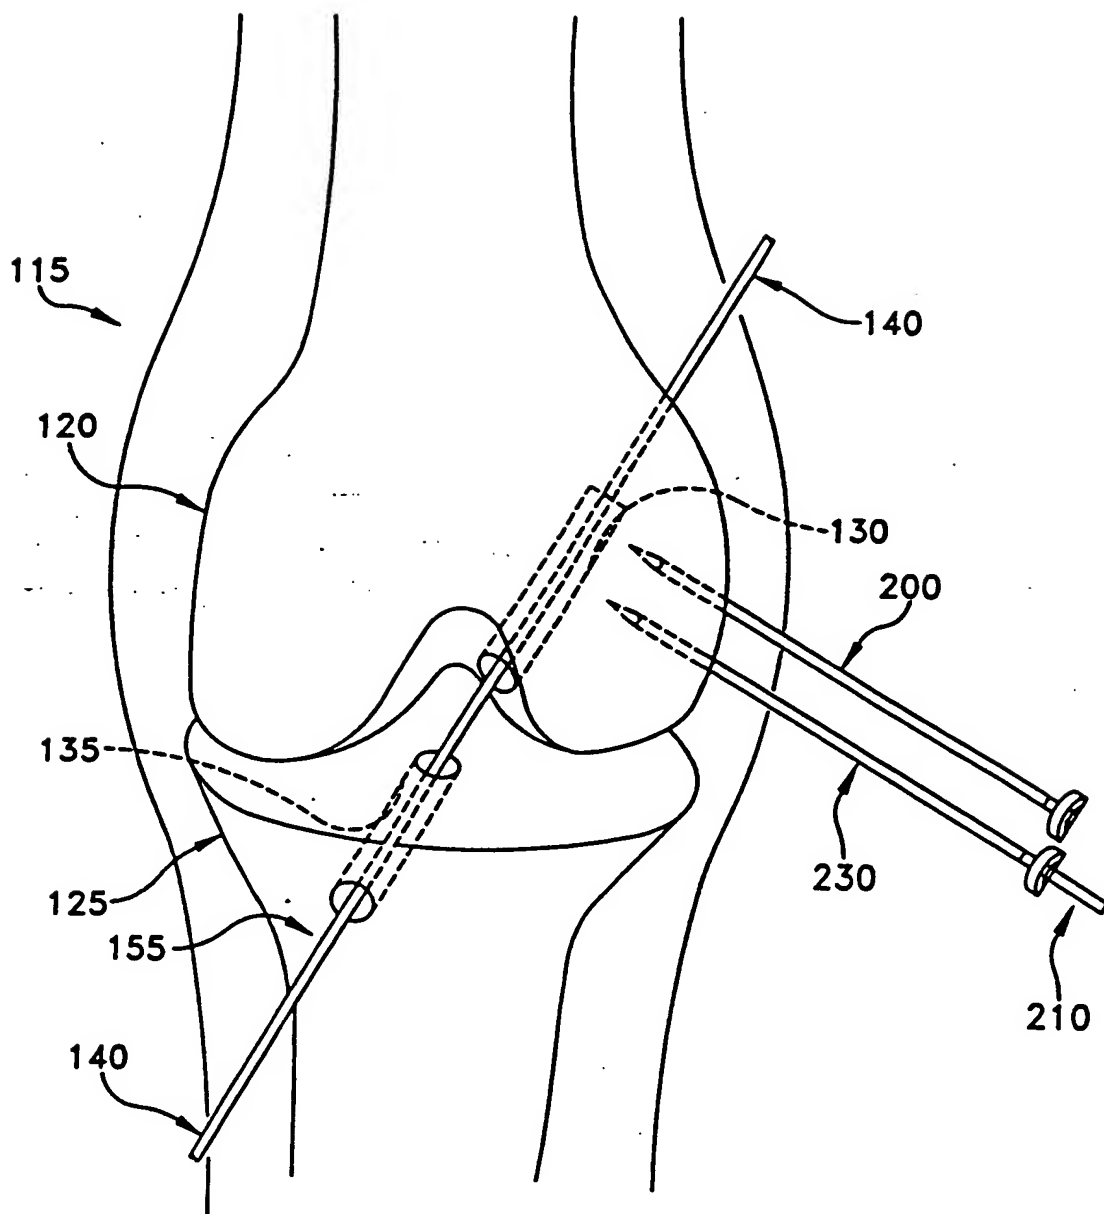


FIG. 18

10039857.102601

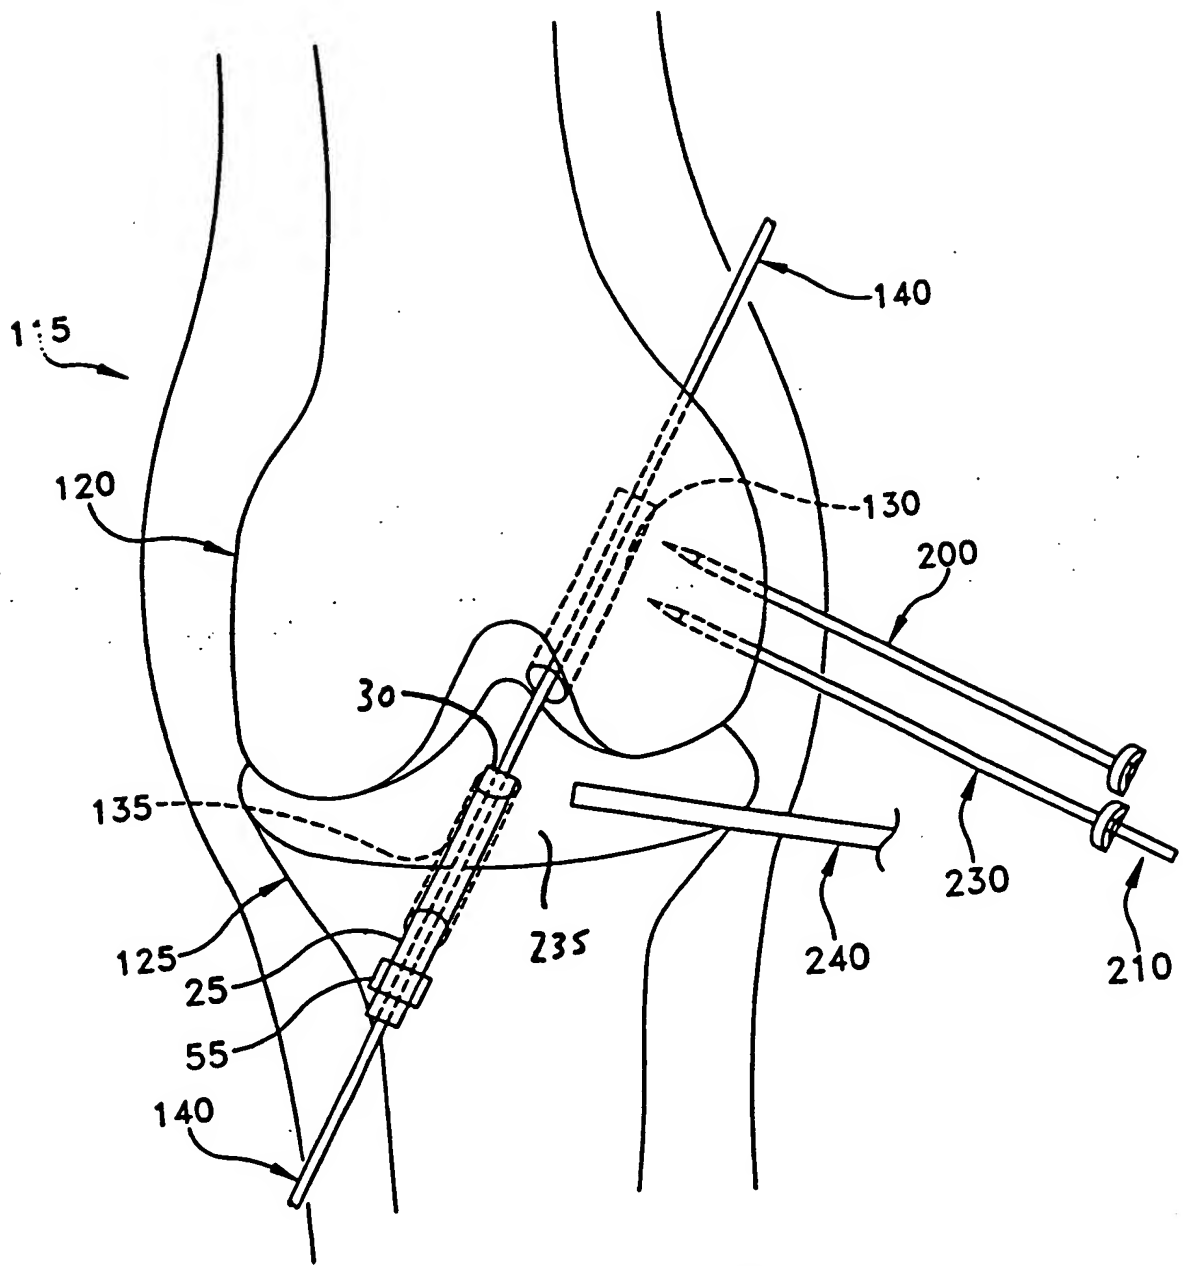


FIG. 19

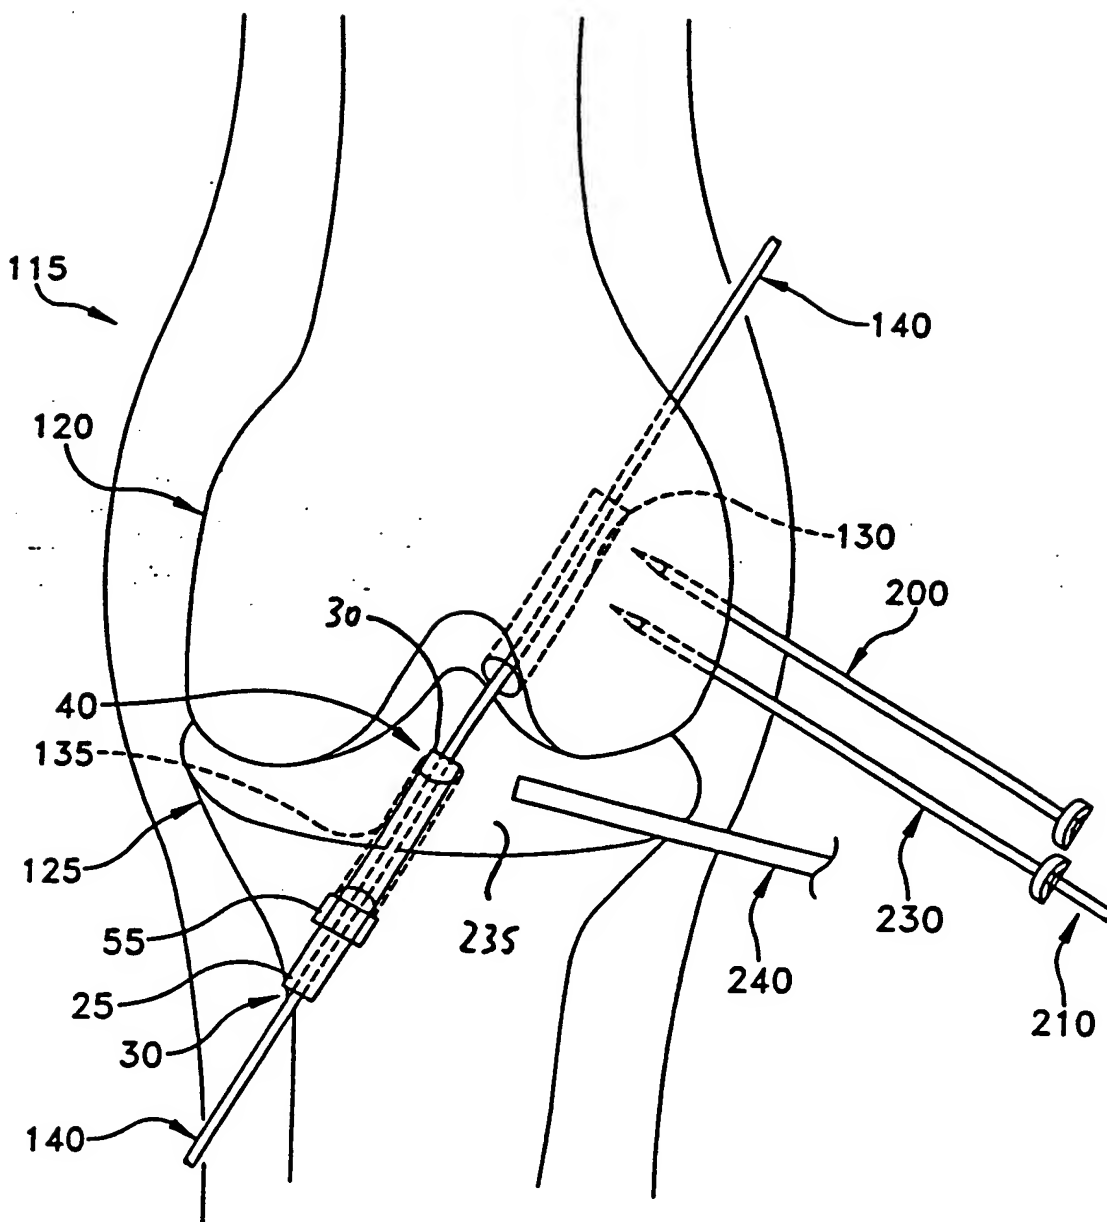


FIG. 20



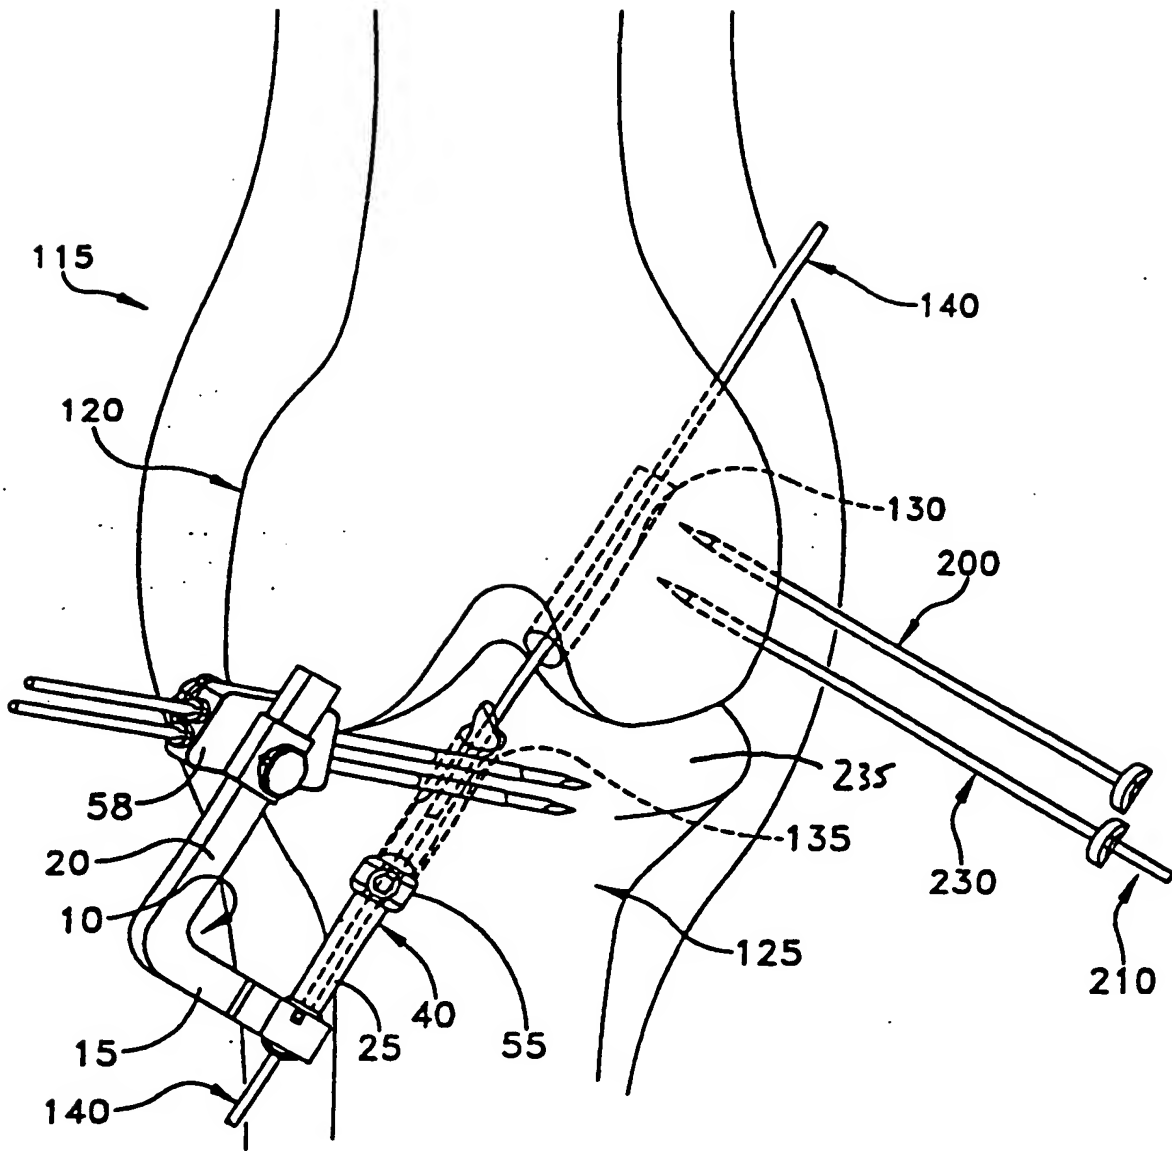


FIG. 21

FIG. 22

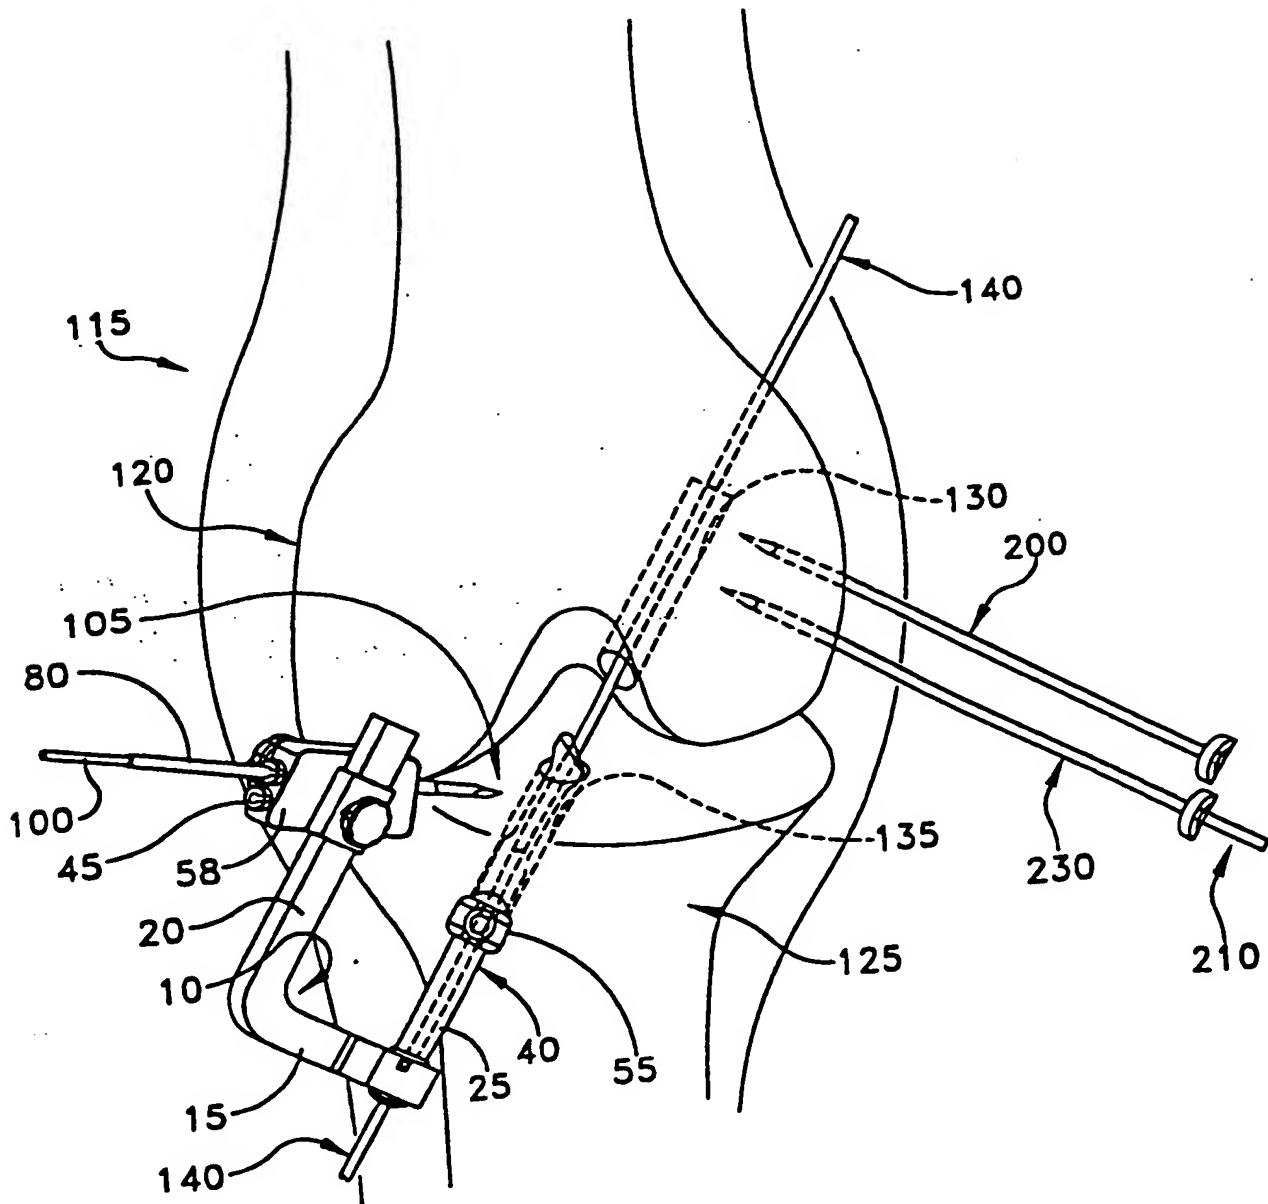


FIG. 22

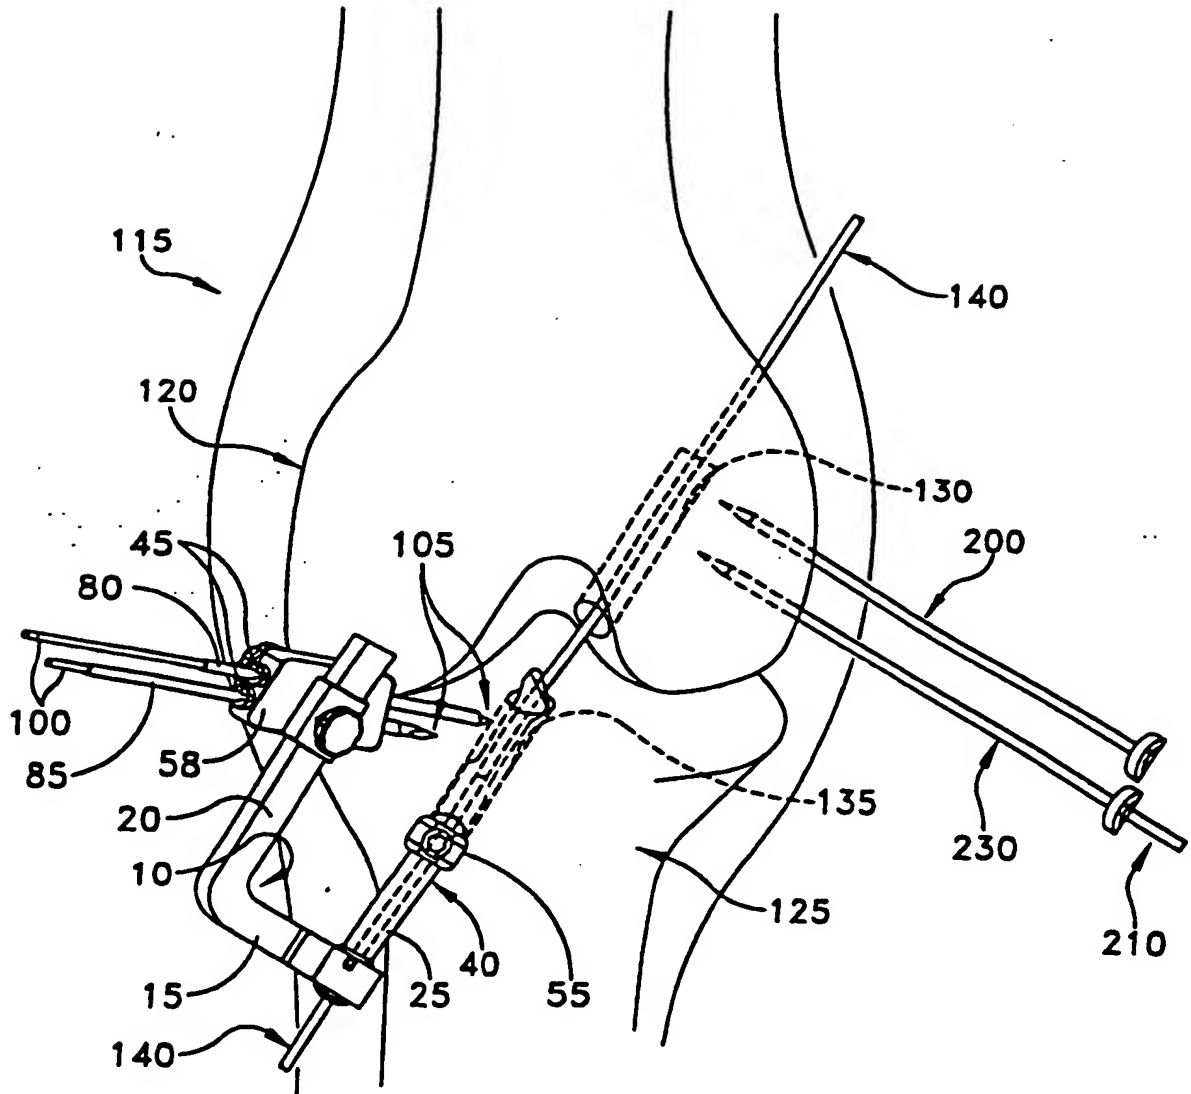


FIG. 23

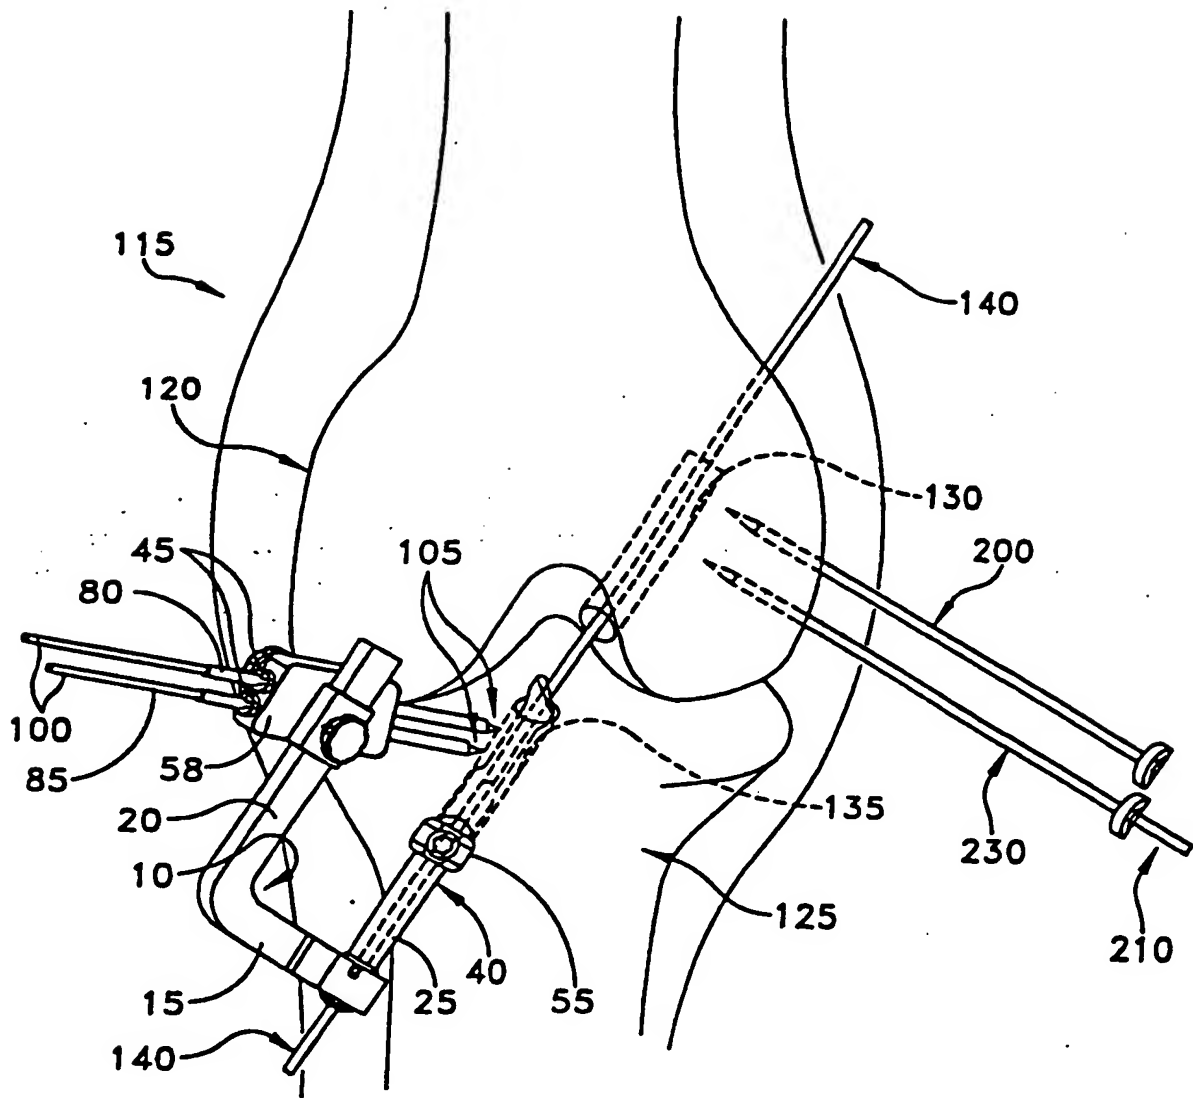


FIG. 24

FIG. 25

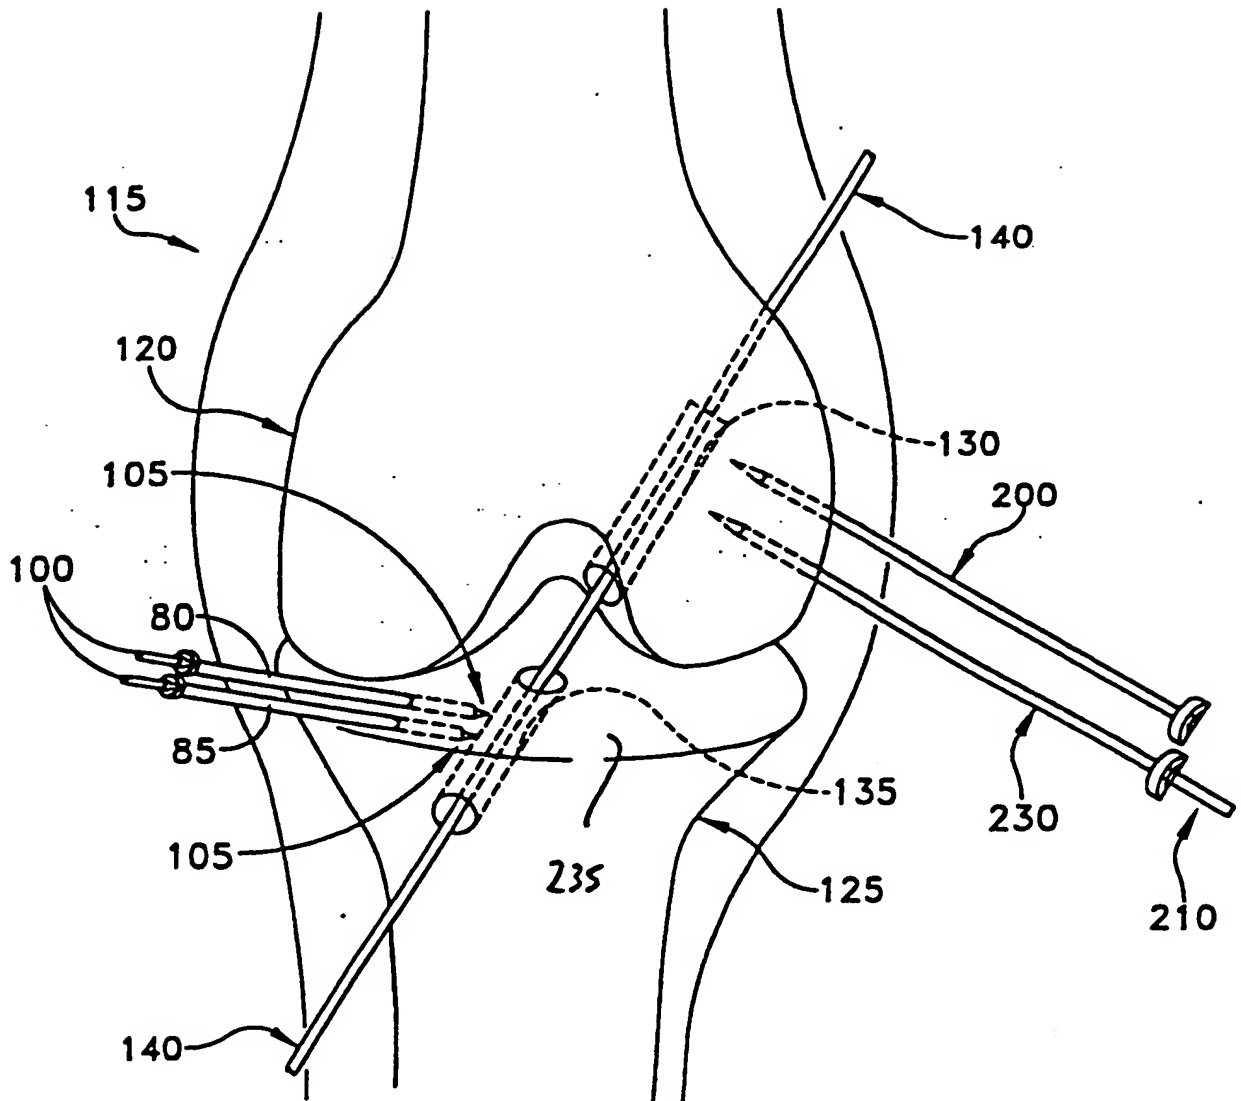


FIG. 25

FIG. 1 is a schematic diagram of a medical device 100 implanted in a patient's body. The device includes a main shaft 115 with a proximal handle 120 and a distal tip 140. A tensioning cable 200 is connected to the distal tip and extends through the body to a handle 210. The cable is secured by a locking mechanism 230. A dashed line 130 indicates the intended path of the cable. Other components labeled include 80, 85, 105, 125, 135, 165, 235, and 250.

**FIG. 26**

10039852 102601

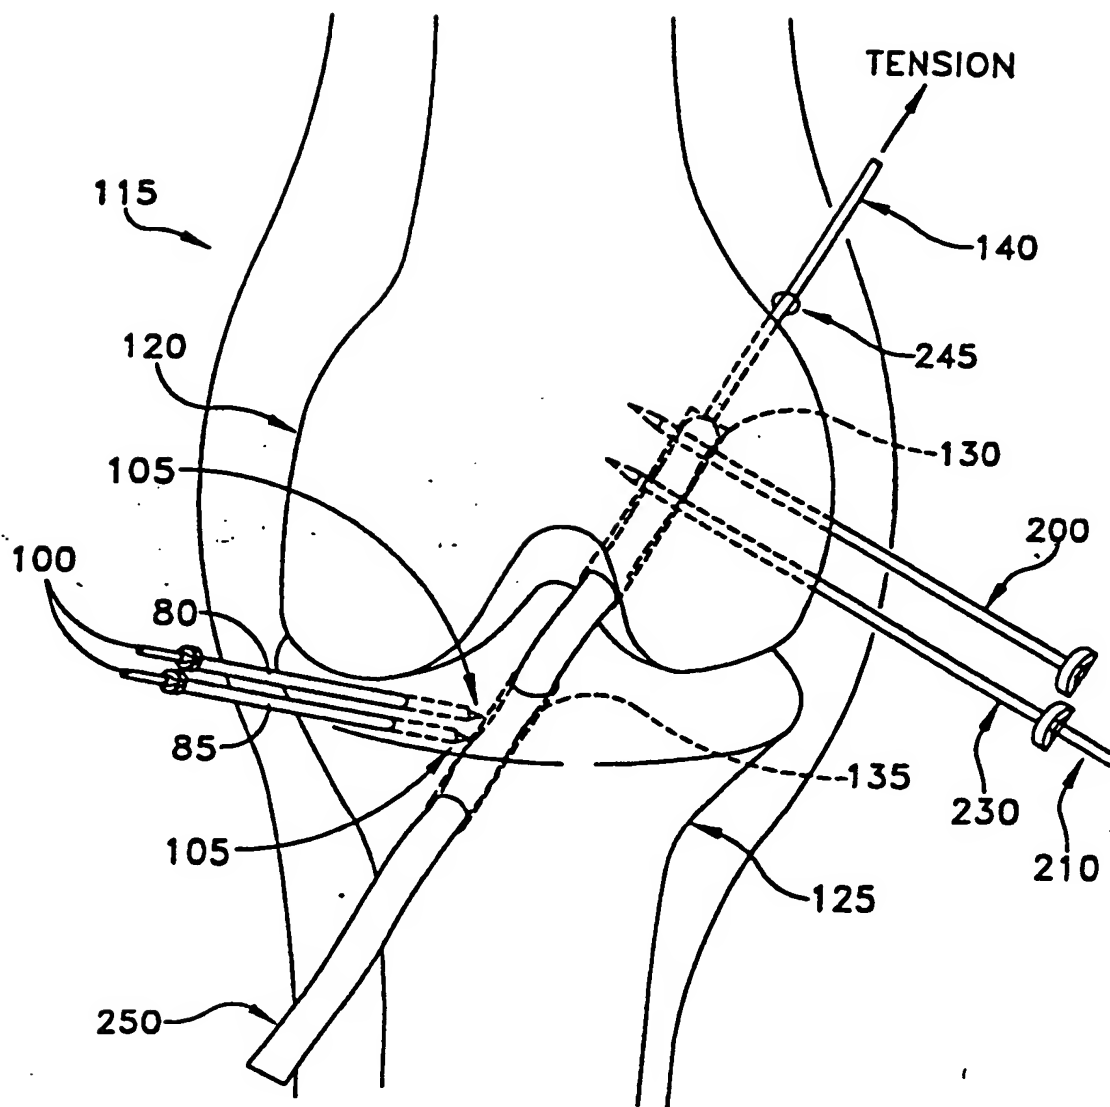


FIG. 21

FIG. 28

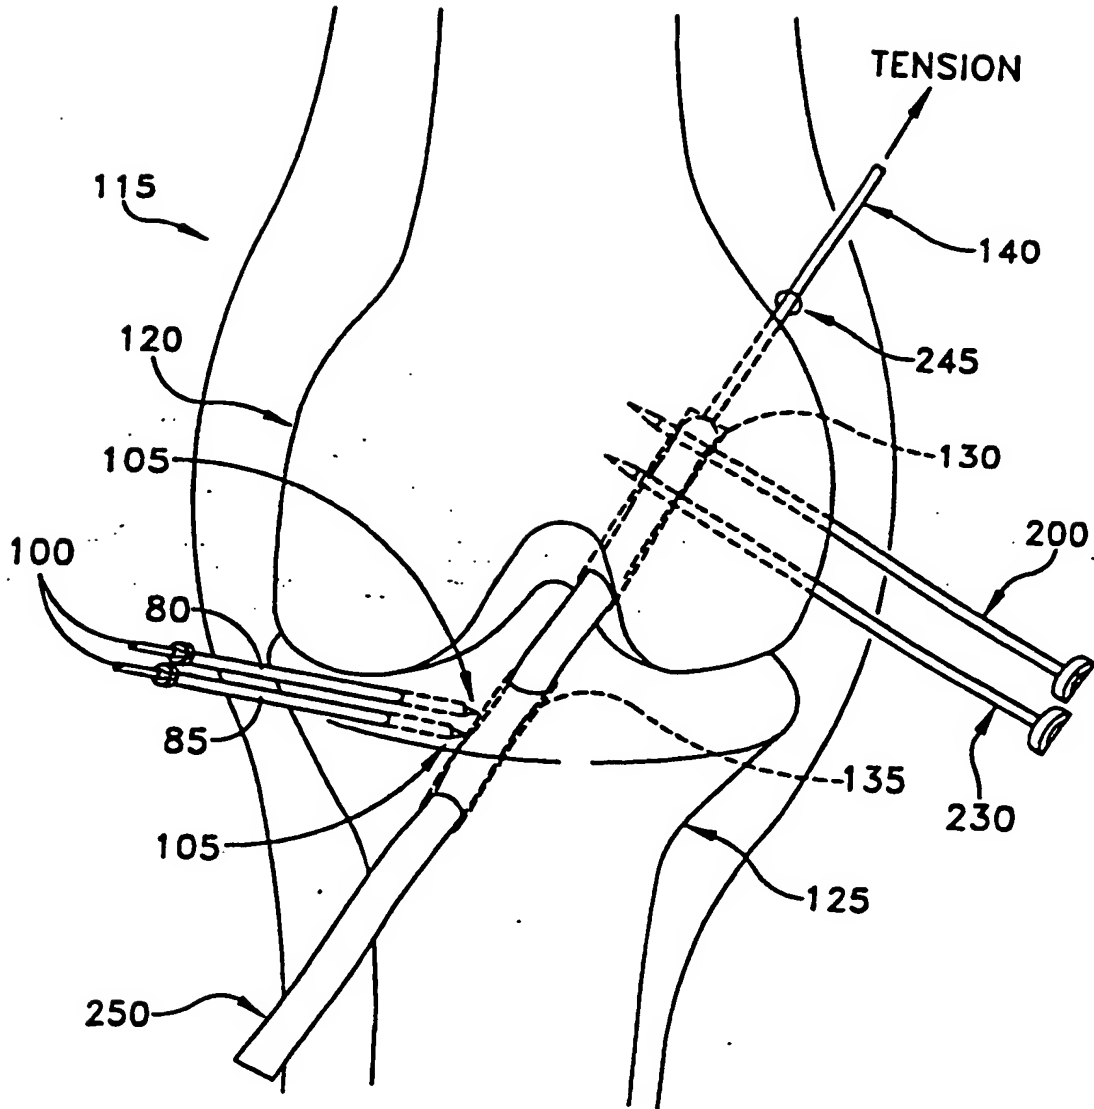


FIG. 28



FIG. 29

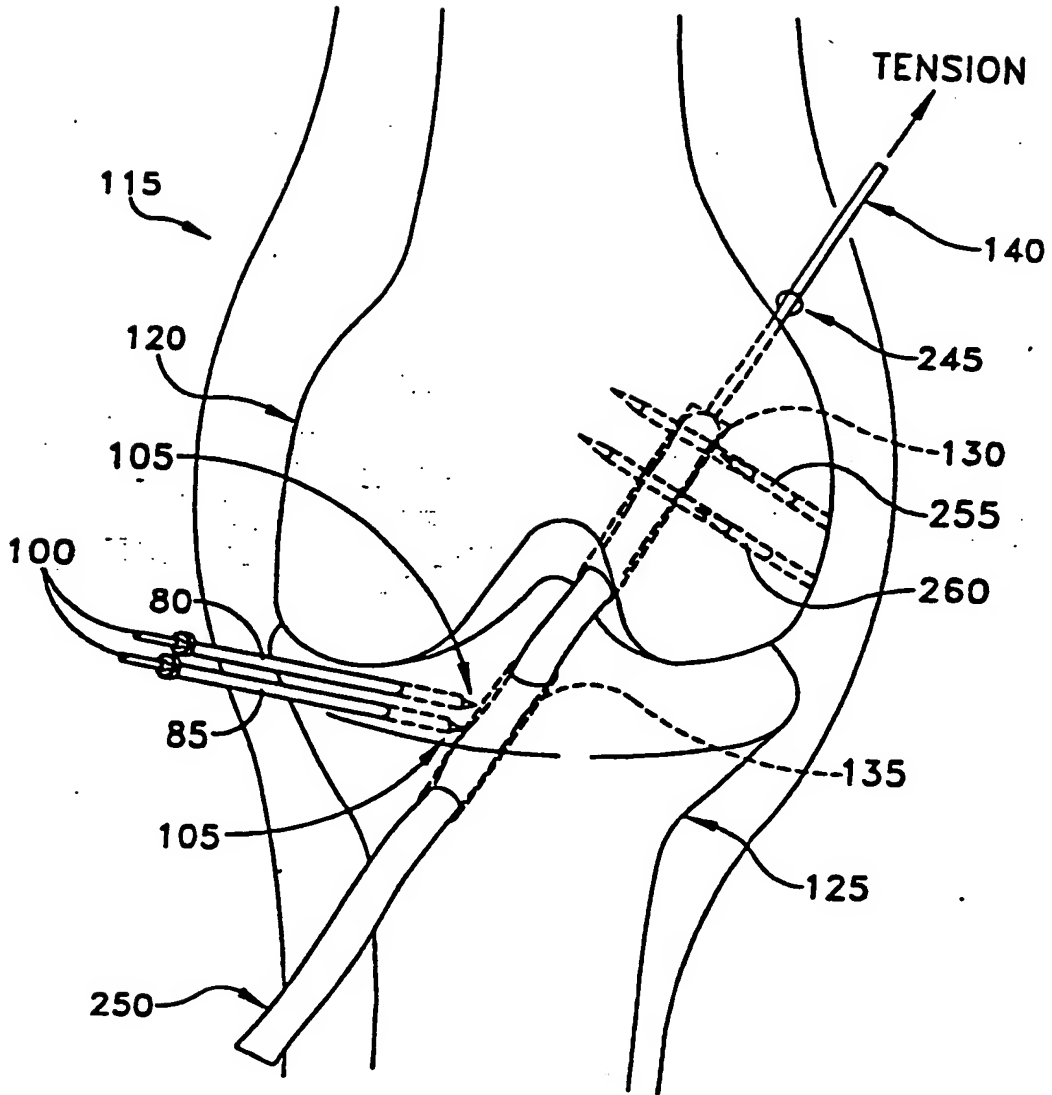


FIG. 29

10039857-102601

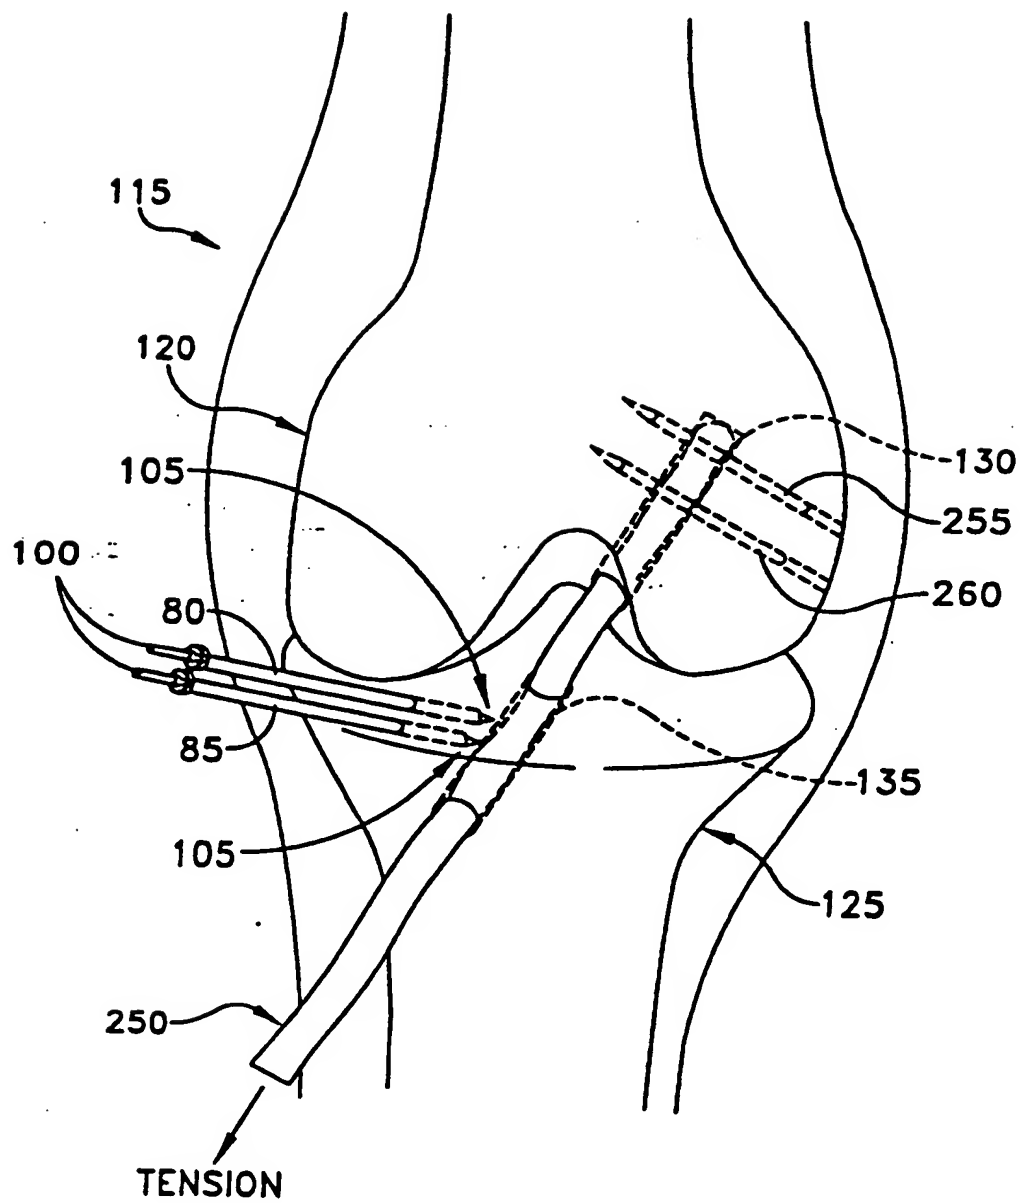


FIG. 30

10039857.102601

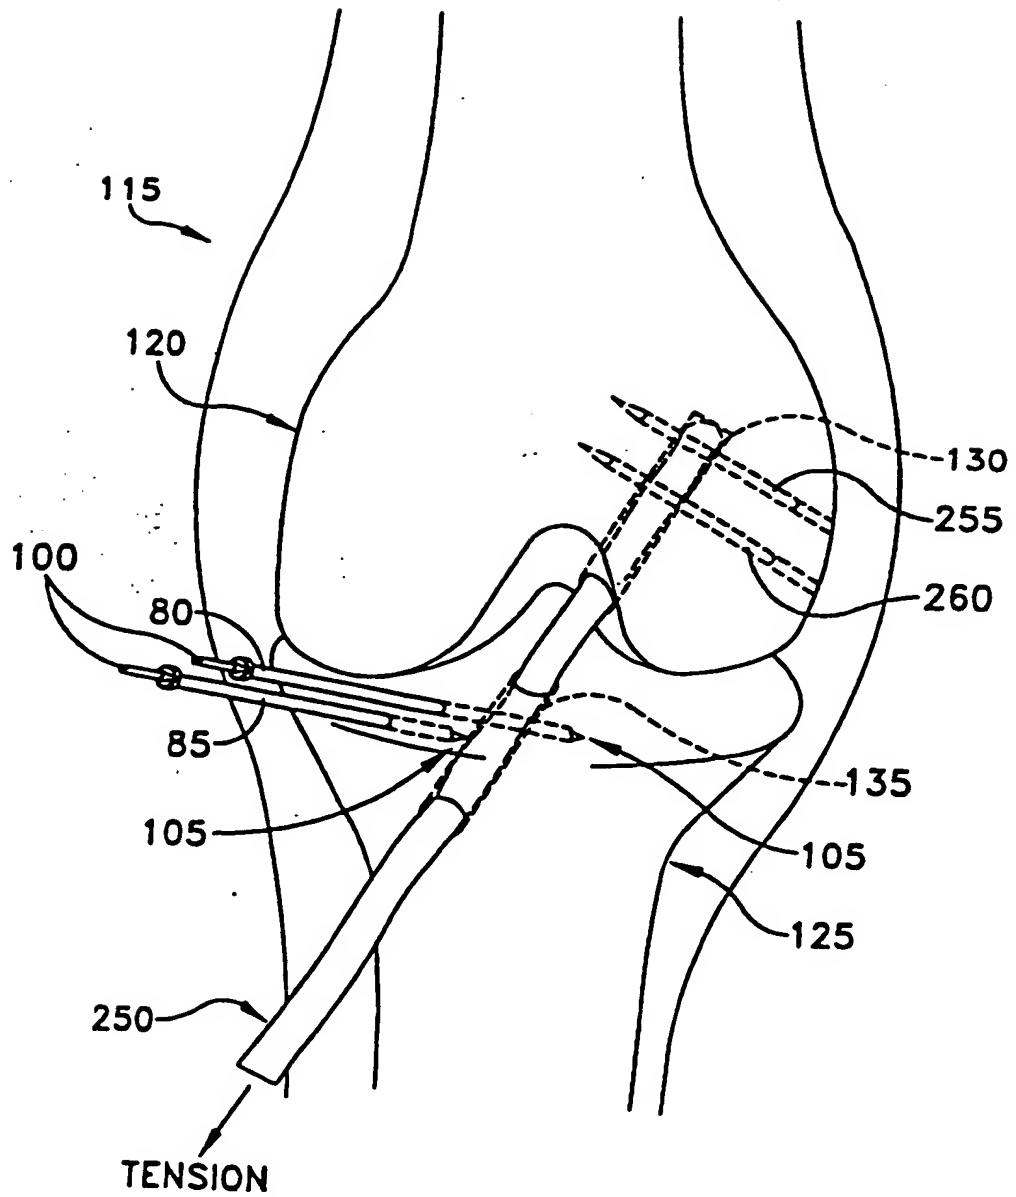


FIG. 31

FIG. 32

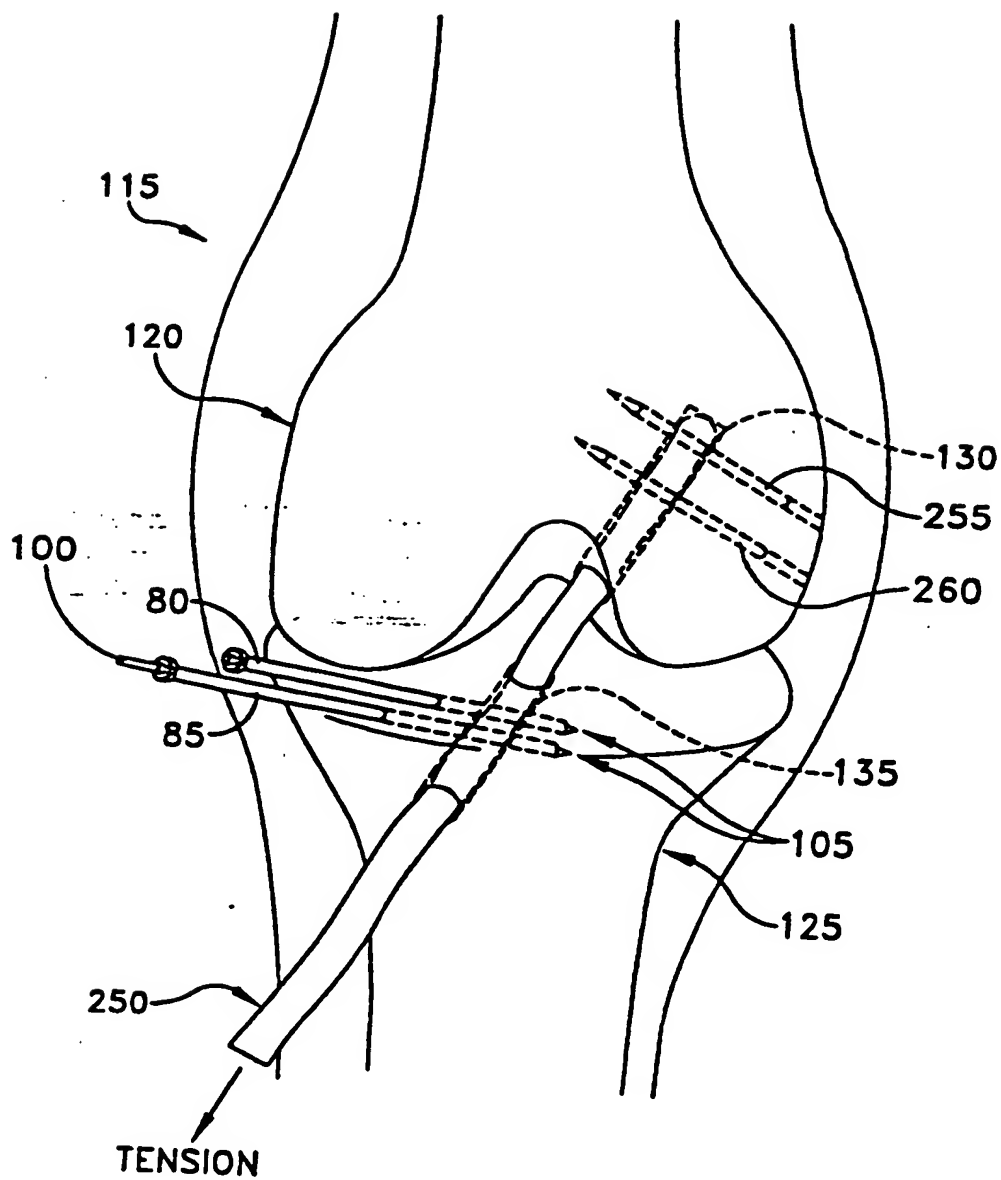


FIG. 33

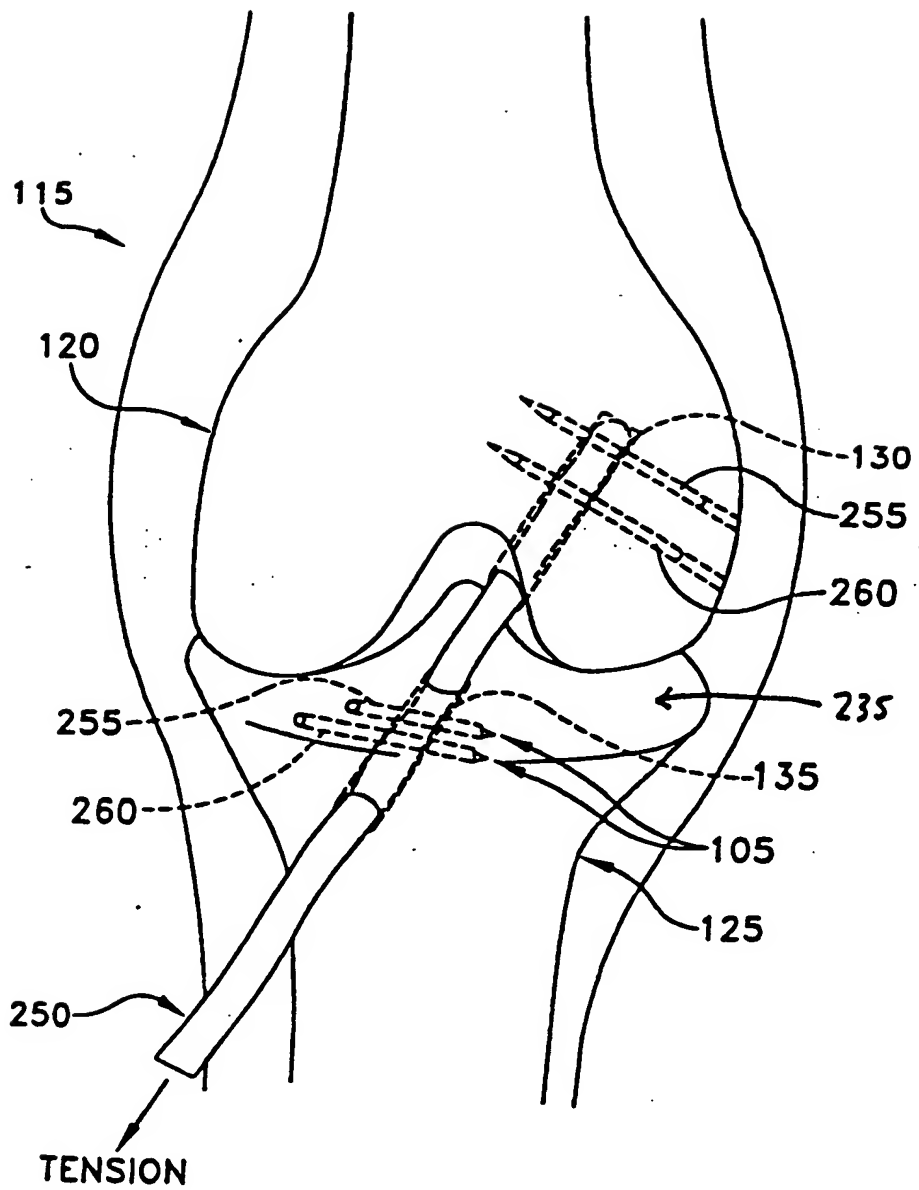
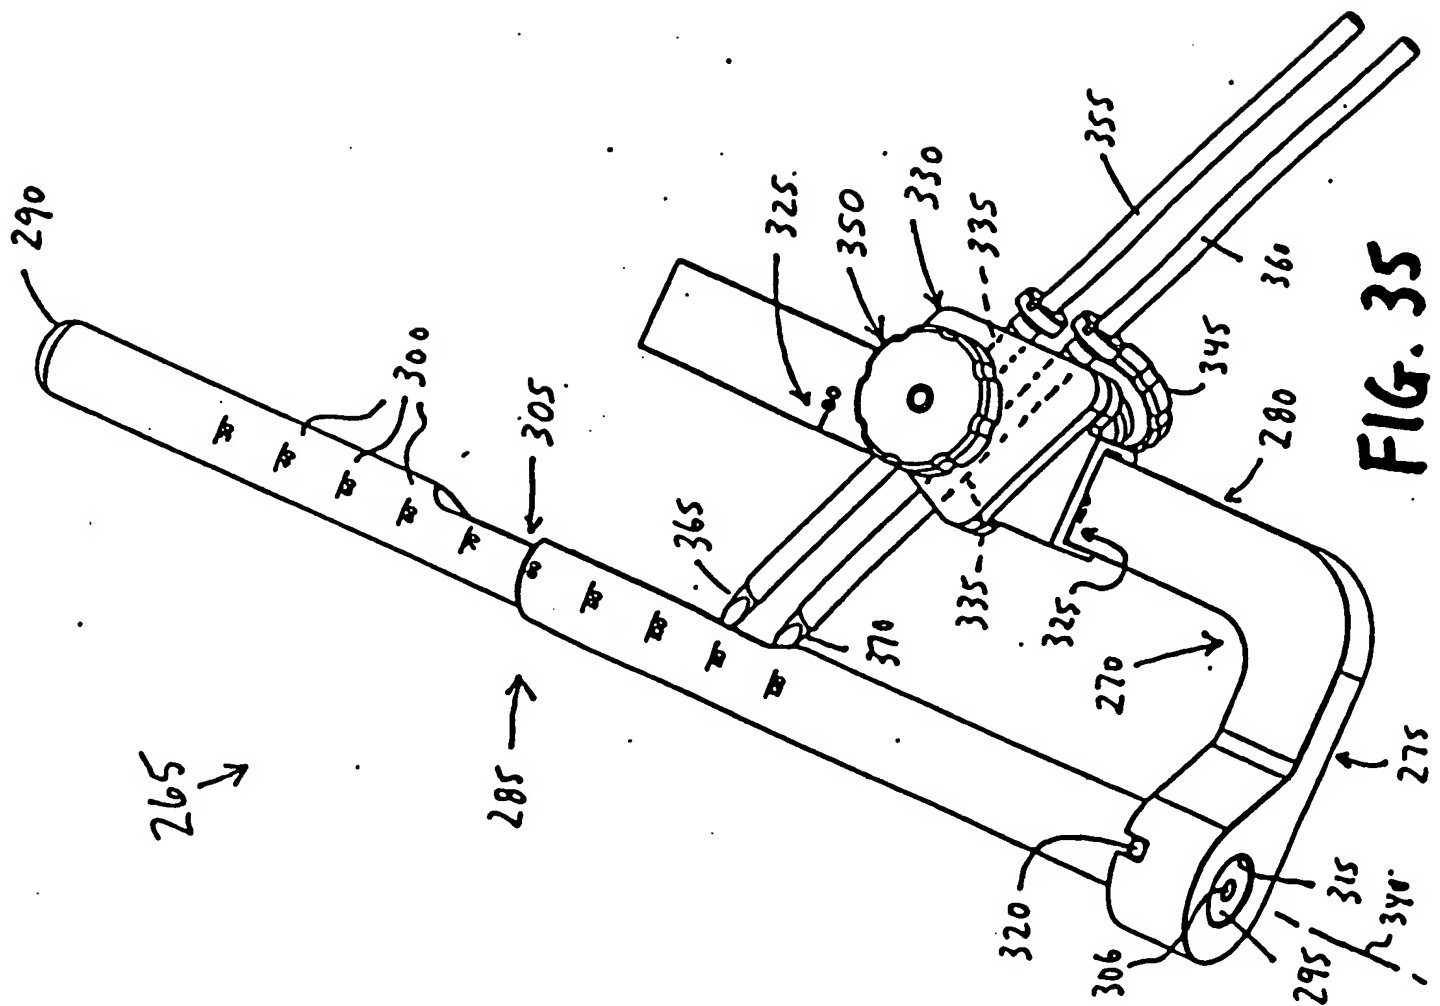


FIG. 34

FIG. 36



**FIG. 35**

FIG. 38

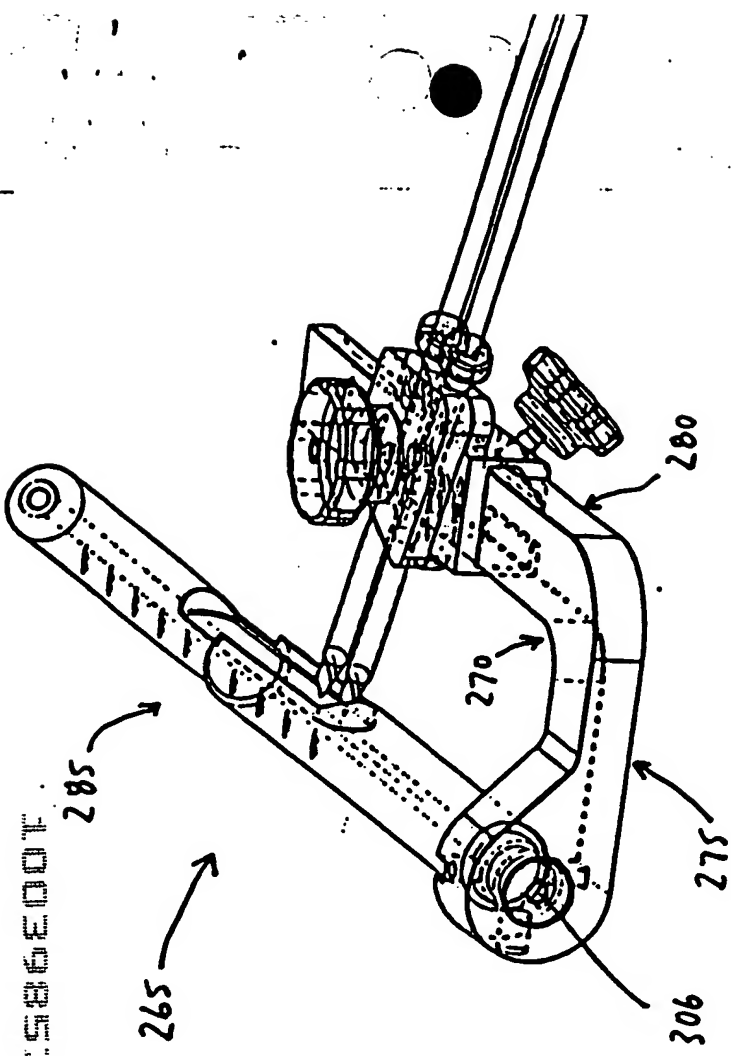


FIG. 38

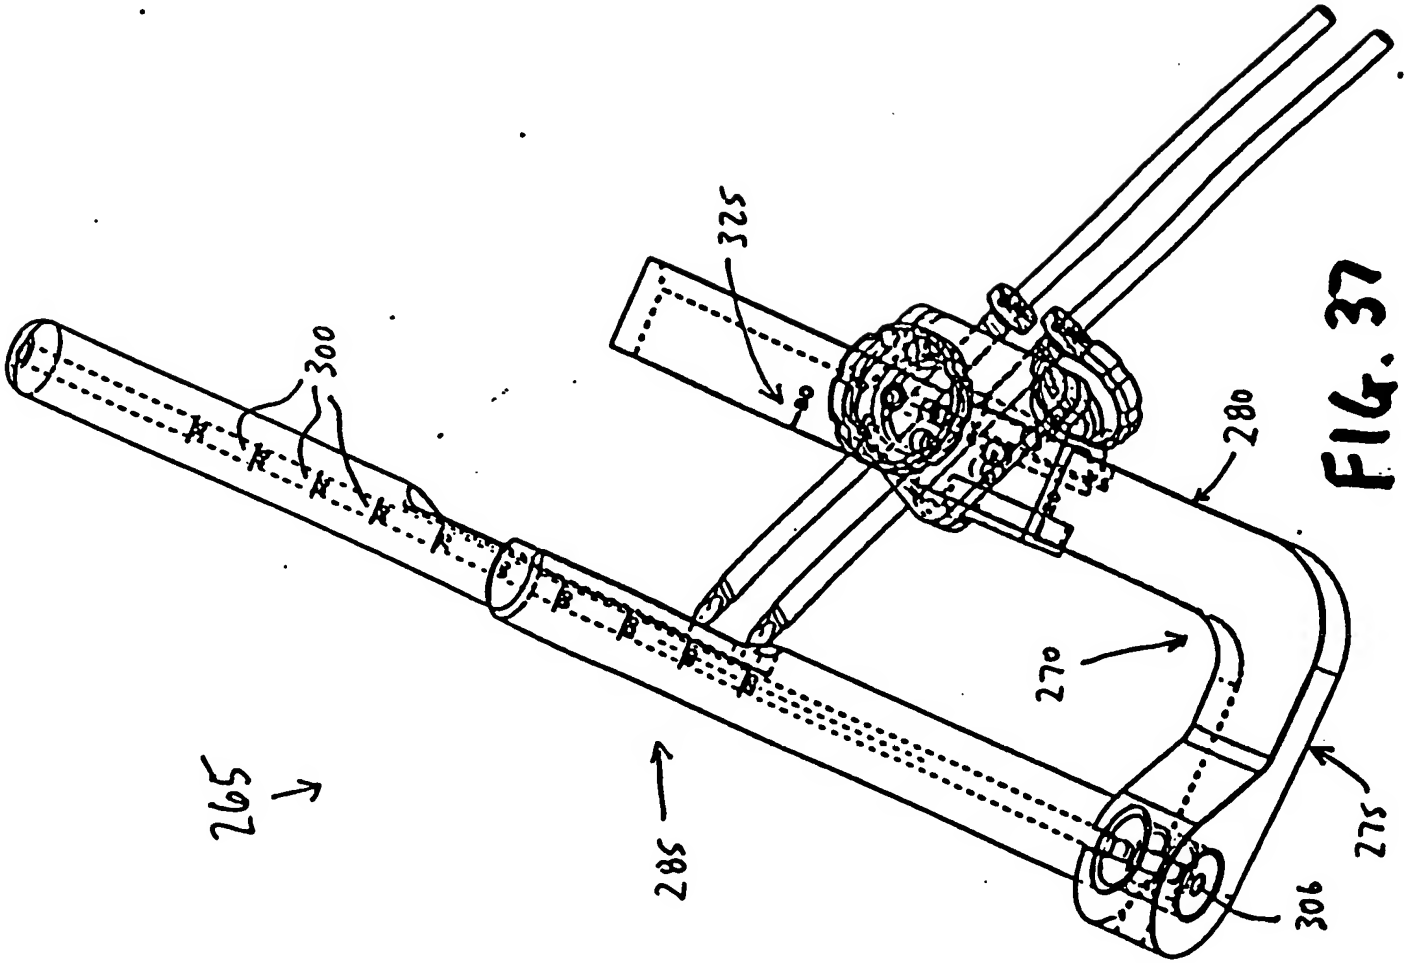


FIG. 37



10039855-102601



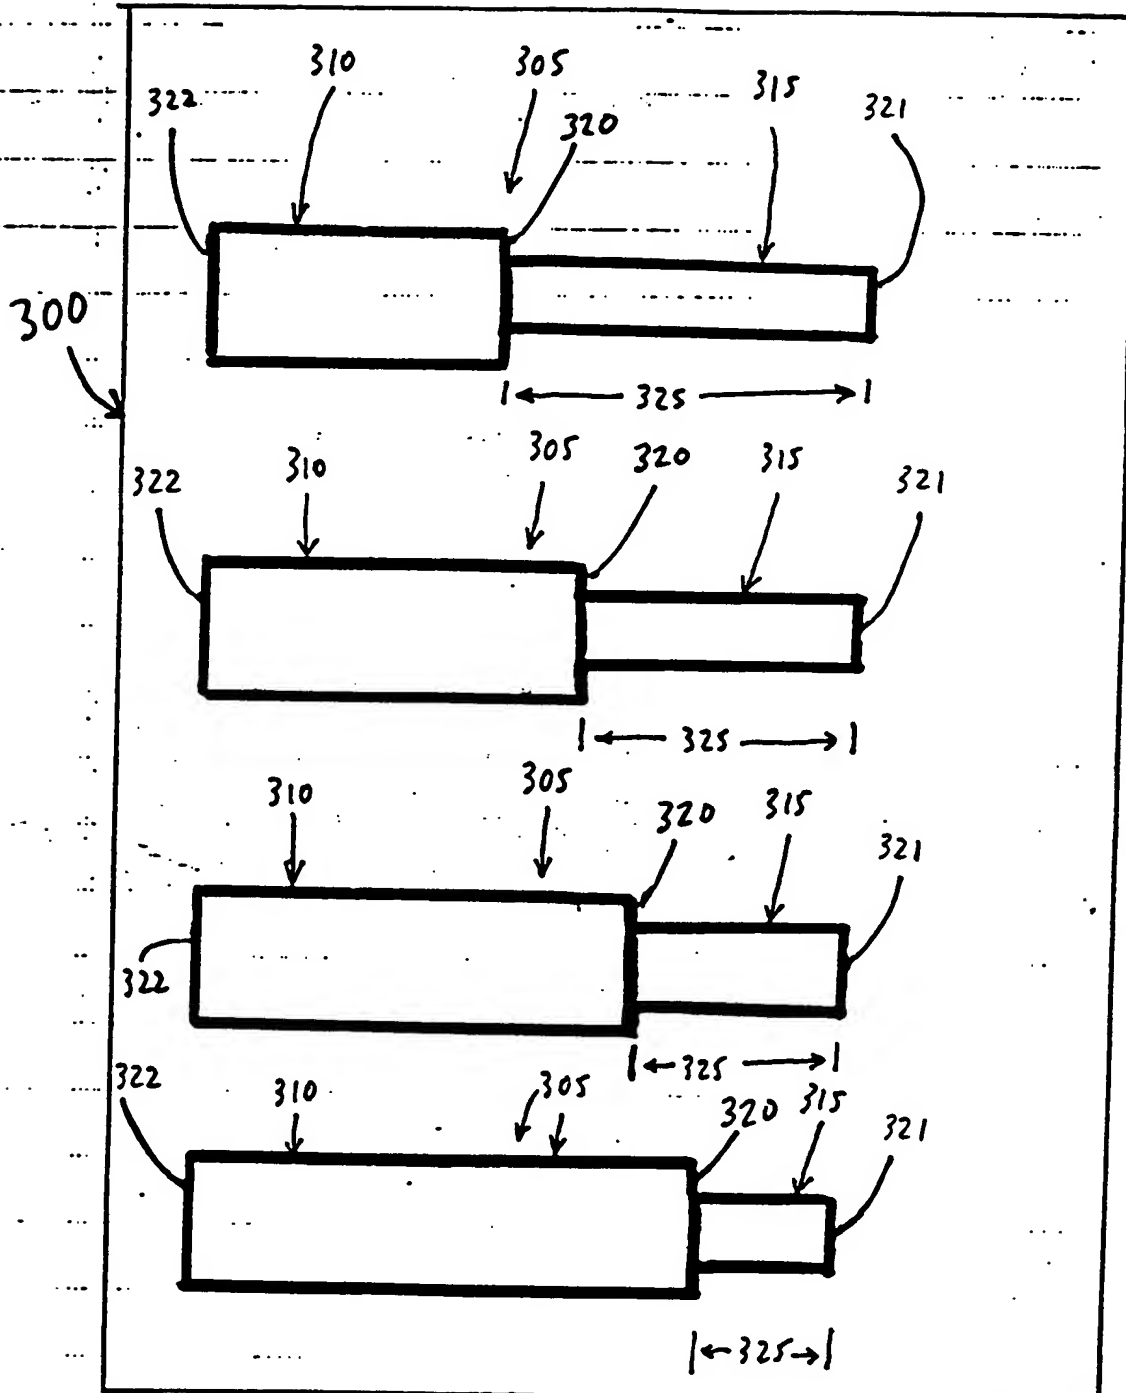


FIG. 39



;

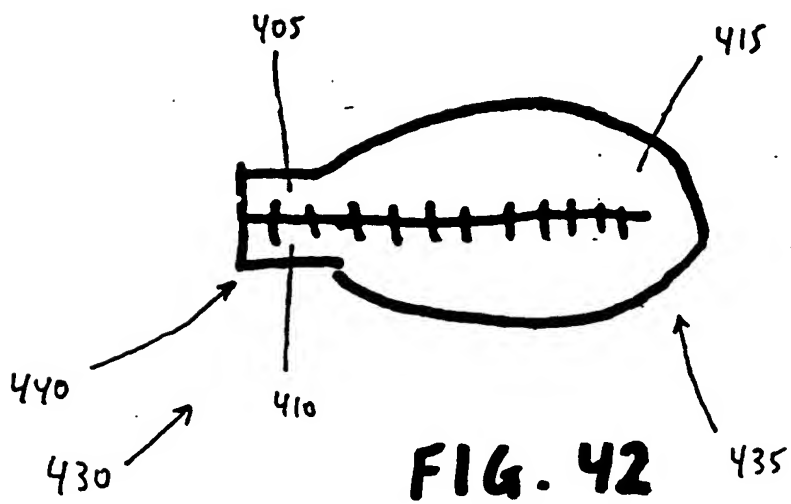

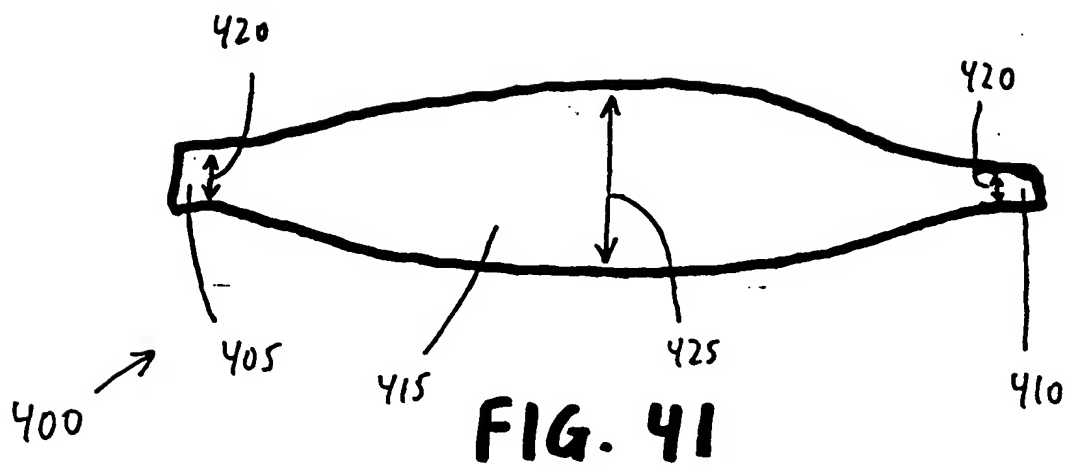

10039857 "102601

10039857-102601

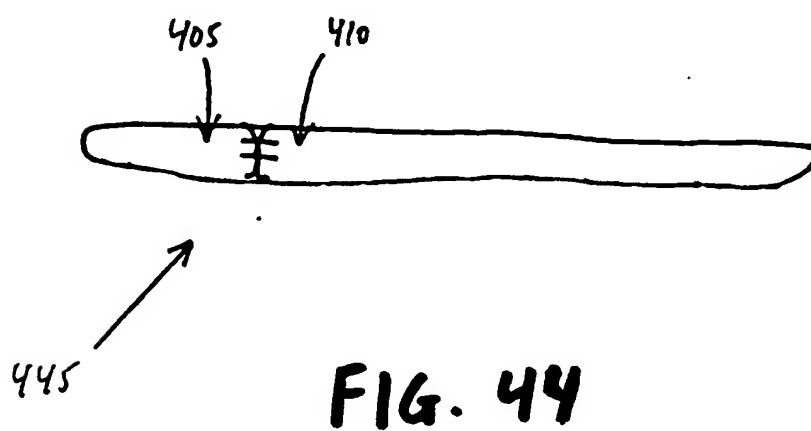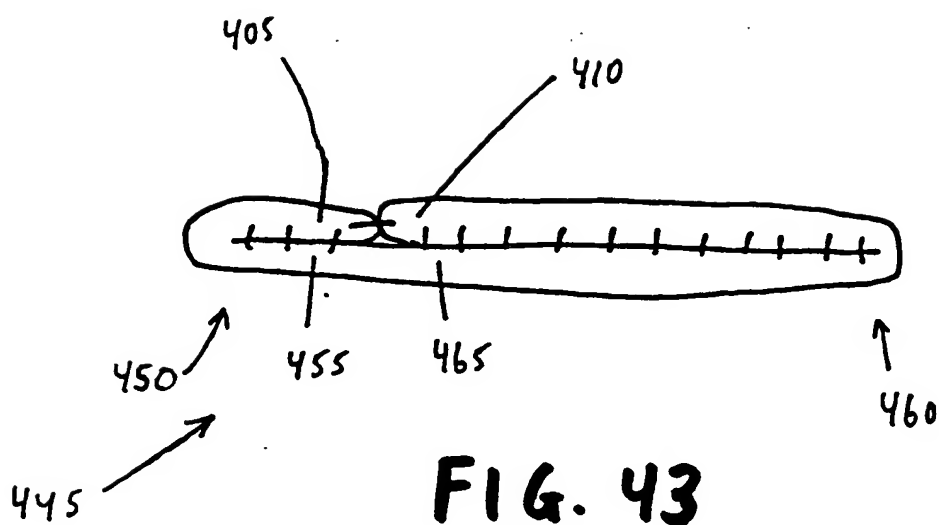

10039857-10601

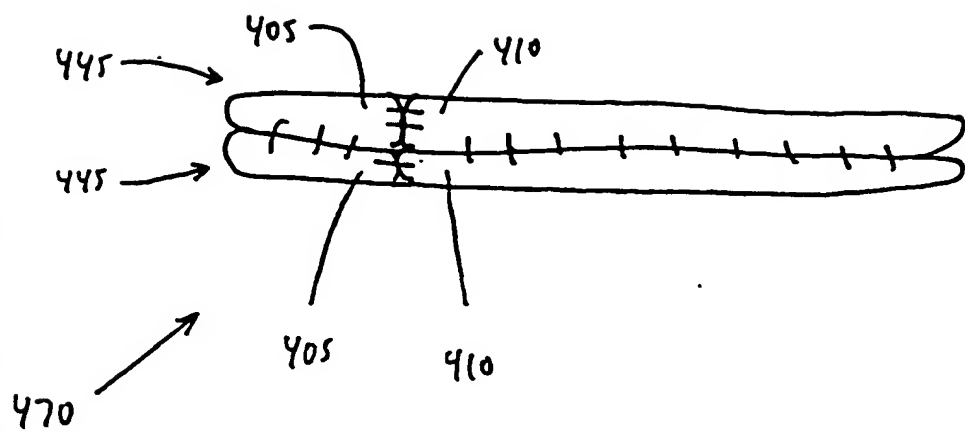


FIG. 45

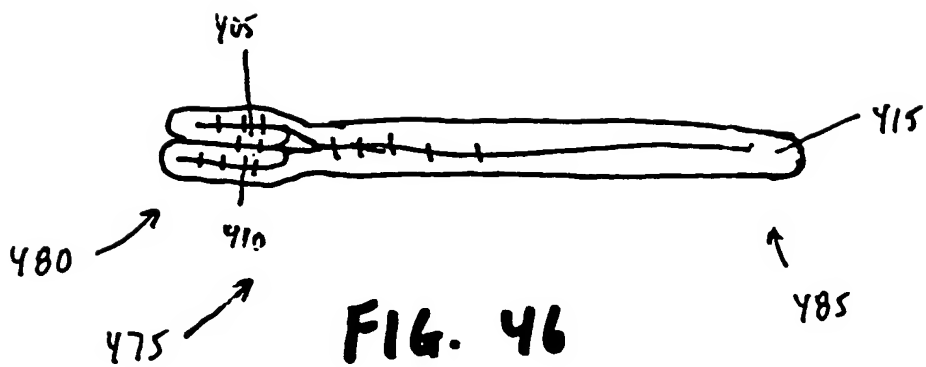


FIG. 46

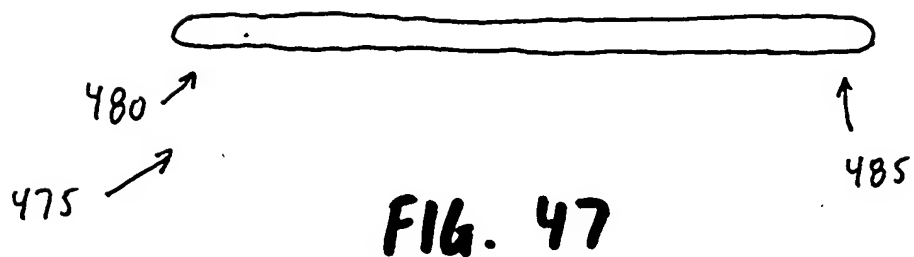


FIG. 47

10039857-102601

10039857-102601

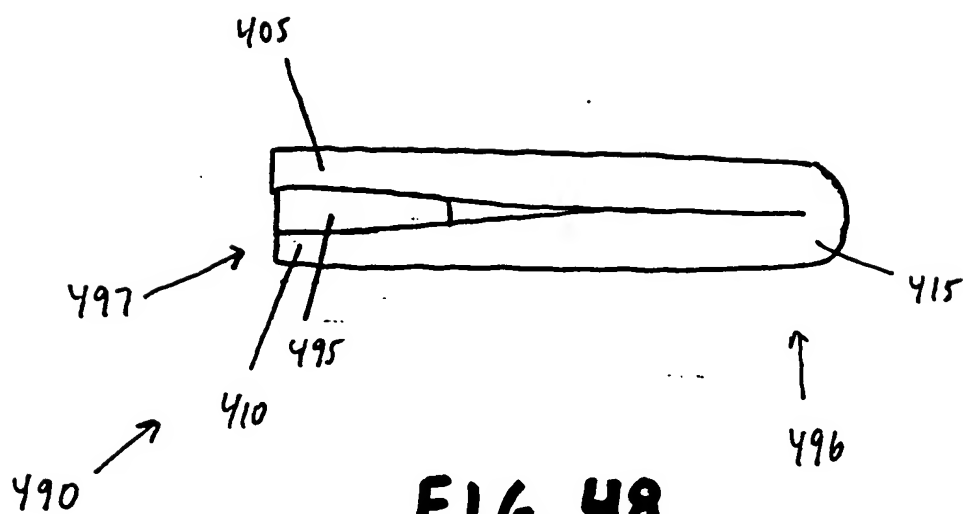


FIG. 48